

2025 Q4 SENSOR REPORT
COMMERCE CITY NORTH DENVER
COMMUNITY AIR MONITORING NETWORK
COMMERCE CITY, COLORADO

Prepared for: Suncor Energy (U.S.A.) Inc.

Prepared by: Onterris Air Quality Services, LLC, formerly known as Montrose Air
Quality Services, LLC

Onterris Response and Recovery, LLC, formerly known as The
Center for Toxicology and Environmental Health (CTEH), LLC

June 9, 2026

Version 1.0

Document Number: 317AA-049284-RT-1237

Report Period: October 1 – December 31, 2025

Executive Summary

In response to community feedback, Suncor Energy (U.S.A.) Inc. (Suncor) voluntarily developed an air monitoring program to gain insight into air quality for neighborhoods in the vicinity of Suncor's operations in Commerce City, Colorado, in 2021. On December 31, 2024, Suncor became required to conduct community monitoring pursuant to CRS § 25-7-146(3)(a). Suncor, however, voluntarily engaged a third-party consultant to perform health risk assessments and publish reports of its monitoring results online. Onterris - Air Quality Services, LLC operates the air monitoring network in the Commerce City and North Denver (CCND) neighborhoods, and health scientists from Onterris Response and Recovery, LLC, perform a screening-level human health risk assessment. A screening-level assessment compares exposure concentrations (ECs) to reference levels (RLs) set by state and/or federal guidance that represent exposure levels that protect public health and the environment.

Air monitoring under the program is continuous and near real-time, and uses three separate technical approaches:

1. Continuous, near real-time air monitoring for the following compounds using sensor technology: carbon monoxide (CO), sulfur dioxide (SO₂), hydrogen sulfide (H₂S), nitrogen dioxide (NO₂), particulate matter (PM_{2.5}), total volatile organic compounds (tVOCs), benzene, toluene, ethylbenzene, and xylenes;
2. Periodic (planned and triggered) air sample collection and laboratory analysis for the presence of 59 VOCs from evacuated canisters (colloquially referred to as "Summa" canisters); and
3. Periodic real-time air monitoring throughout six neighborhoods using a mobile monitoring van to detect the presence of 65 chemicals that are evaluated as 18 individual chemicals with the remaining 47 chemicals being combined into 12 chemical groups known as isomer groups.

This report details the first approach, which uses continuous air monitoring sensors operating at 10 locations across the CCND neighborhoods. Preliminary air monitoring data is made available in near real-time at ccnd-air.com, and this report analyzes the final data collected between October 1 – December 31, 2025. The data are processed and averaged to match the same time intervals as established health-based reference levels, where available, and then compared to these reference levels to evaluate concentration trends over time. Unlike the second and third approach listed above, these sensor data are not used in a human health risk assessment or calculation of exposure metrics. Instead, this sensor report provides information on concentration trends for the given quarter.

The results of the air monitoring data conducted in Q4 of 2025 indicate the following:

- For all compounds except benzene (24-hour rolling average), rolling and/or block average concentrations fell below their respective health-based reference levels (RLs).

- The 24-hour rolling average concentrations of benzene was above the Agency for Toxic Substances and Disease Registry (ATSDR) Acute MRL (9 ppb) at CM1 on October 2 (9.34 – 9.80 ppb) and October 14 (9.26 – 13.32 ppb), 2025. Notably, the CM1 BTEX sensor showed an elevated baseline and kept failing the bump test for all BTEX compounds beginning on September 29, 2025. Therefore, it was determined that the BTEX sensor had a malfunctioning PID source, which resulted in an elevated baseline and could potentially be the reason for these higher benzene concentrations. The system was serviced and the PID source was replaced on October 16, 2025, after which the baseline decreased.
- No valid H₂S and SO₂ measurements were collected at CM6 during Q4 2025 given that the monitor at this location failed weekly QC tests. The team determined that a faulty UV lamp caused the instrument baseline to gradually increase each week and then decrease following the weekly calibration sequence, resulting in invalid measurements. The UV lamp was replaced during Q1 2026.
- During a total of four trigger events, the tVOC 1-minute measurements exceeded the 1 ppm threshold and triggered the collection of four canister samples. The results of these triggered canister analyses will be available in a separate report at <https://www.ccnd-air.com/>.

Table of Contents

1.0	Introduction.....	1
2.0	Methods	1
2.1	Air Monitoring Site Description	1
2.2	Continuous Monitoring.....	3
2.3	Assessment of Real-Time Air Monitoring Trends	6
3.0	Results	7
3.1	Results Summary	7
4.0	Program changes.....	23

List of Figures

Figure 1	Map of 10 CCND Monitor Locations	2
Figure 2	CCND Community Monitoring Carbon Monoxide (CO) 1-Hour Rolling Average Data....	10
Figure 3	CCND Community Monitoring Nitrogen Dioxide (NO ₂) 1-Hour Rolling Average Data	11
Figure 4	CCND Community Monitoring Sulfur Dioxide (SO ₂) 1-Hour Rolling Average Data.....	12
Figure 5	CCND Community Monitoring Hydrogen Sulfide (H ₂ S) 1-Hour Rolling Average Data....	13
Figure 6	CCND Community Monitoring Hydrogen Sulfide (H ₂ S) 24-Hour Rolling Average Data..	14
Figure 7	CCND Community Monitoring PM _{2.5} 1-Hour Block Average Data	15
Figure 8	CCND Community Monitoring PM _{2.5} 24-Hour Block Average Data	16
Figure 9	CCND Community Monitoring tVOC 1-Hour Rolling Average Data.....	17
Figure 10	CCND Community Monitoring Benzene 1-Hour Rolling Average Data	18
Figure 11	CCND Community Monitoring Benzene 24-Hour Rolling Average Data.....	19
Figure 12	CCND Community Monitoring Ethylbenzene 1-Hour Rolling Average Data	20
Figure 13	CCND Community Monitoring 1-Hour Rolling Average Toluene Data.....	21
Figure 14	CCND Community Monitoring 1-Hour Rolling Average Xylene Data	22

List of Tables

Table 1	CCND Monitors and Summa Canister Sampling Locations SAMPLING.....	3
Table 2	CCND Air Monitoring Technology.....	4
Table 3	CCND Monitors Results Summary.....	9

▸ Appendices

- Appendix A Calibration and QA/QC Data
- Appendix B Field Data Sheets
- Appendix C Calibration Gas Certification Sheets

1.0 Introduction

In response to community feedback received by Suncor Energy (U.S.A.) Inc. (Suncor) during community engagement that was conducted in the fall of 2020, Suncor voluntarily developed a continuous, near real-time air monitoring program to gain insight into the air quality for neighborhoods in the vicinity of Suncor's operations in Commerce City, Colorado, in 2021. On December 31, 2024, Suncor became required to conduct community monitoring pursuant to CRS § 25-7-146(3)(a). Suncor, however, voluntarily engaged a third-party consultant to perform health risk assessments and publish reports of its air monitoring results online. Onterris - Air Quality Services, LLC was contracted by Suncor to deploy, operate, and maintain the network in the Commerce City and North Denver (CCND) neighborhoods, perform screening-level health risk assessments, and publish reports on the air monitoring results online.

Air monitoring was accomplished through three separate technical approaches:

1. Continuous, near real-time air monitoring for the following compounds using sensor technology: carbon monoxide (CO), sulfur dioxide (SO₂), hydrogen sulfide (H₂S), nitrogen dioxide (NO₂), particulate matter (PM_{2.5}), total volatile organic compounds (tVOCs), benzene, toluene, ethylbenzene, and xylenes;
2. Periodic (planned and triggered) air sample collection and laboratory analysis for the presence of 59 VOCs from Summa canisters; and
3. Periodic real-time air monitoring throughout six neighborhoods using a mobile monitoring van to detect the presence of 65 chemicals that are evaluated as 18 individual chemicals with the remaining 47 chemicals being combined into 12 chemical groups known as isomer groups.

This report details the first approach: the continuous, near real-time air monitoring conducted between October 1 – December 31, 2025. The measured concentrations from the continuous, near real-time air monitoring stations were averaged and compared to health-based reference levels established by federal and/or state agencies to evaluate trends over time. Air monitoring, sampling, and analysis for this approach were conducted in accordance with the Quality Assurance Project Plan (QAPP) that can be found online at <https://www.ccnd-air.com/Documents/>.


2.0 Methods

2.1 Air Monitoring Site Description

Continuous air monitoring sensors were installed at ten locations across CCND neighborhoods within a three-mile radius of Suncor operations. Eight of the sensors were installed in July 2021 (CM1-CM8) and two additional sensors were installed in December 2021 (CM9) and March 2022 (CM10), respectively. The monitor locations are shown in Figure 1 and described in Table 1; and were selected based on the following criteria:

- Historical wind pattern data
- Proximity to Suncor operations and other stationary sources not operated by Suncor
- Existing infrastructure, as well as site access and safety
- Community feedback

Figure 1 Map of 10 CCND Monitor Locations

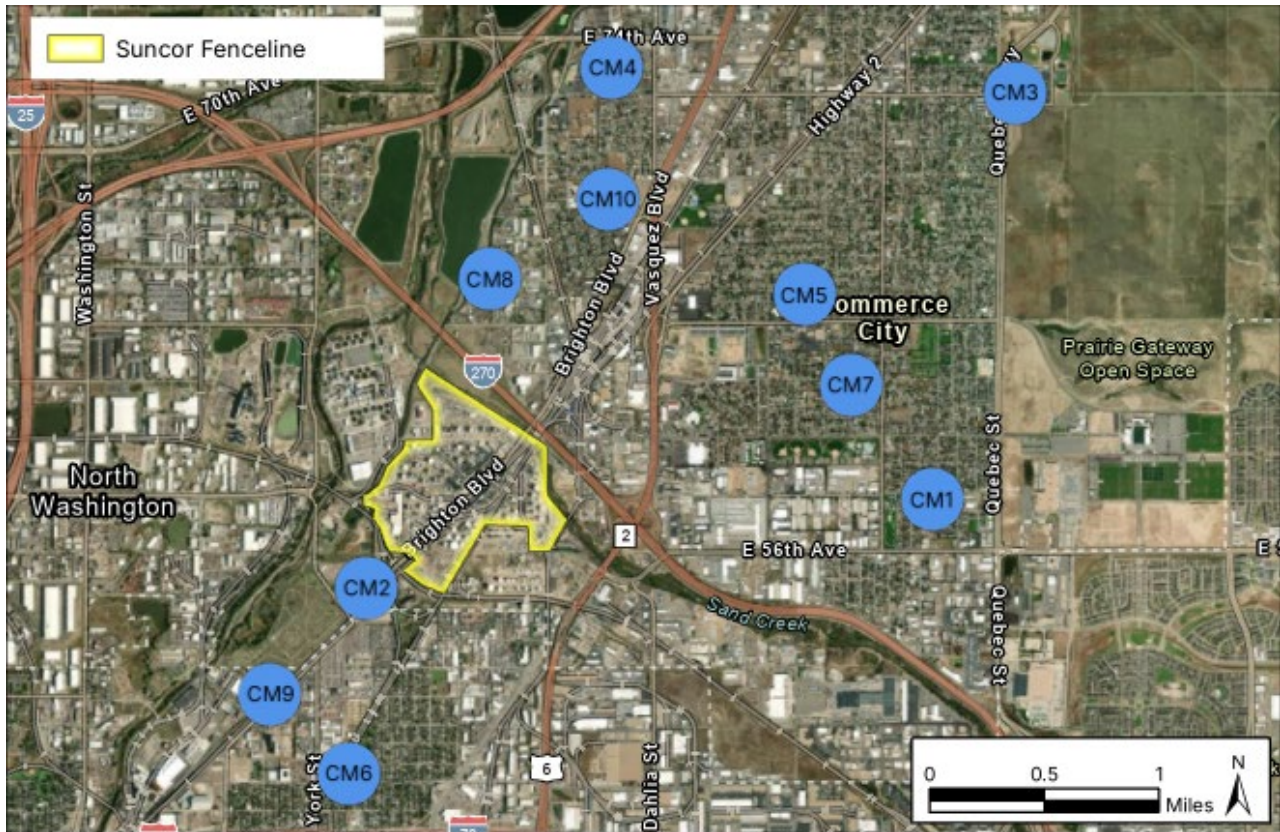

Sources: Esri, TomTom, Garmin, FAO, NOAA, USGS, (c) OpenStreetMap contributors, and the GIS User Community, Vantor

Table 1 CCND Monitors and Summa Canister Sampling Locations

Location ID	Secondary ID	GPS Coordinates	Distance from the Center of Suncor Operations (miles)	Cross Streets
CM1	Rose Hill Elementary School	39.80164, -104.90882	2.0	E. 58 th Ave. & Oneida St., Commerce City
CM2	Suncor Business Center	39.79630, -104.95727	0.70	Brighton Blvd. & York St., Commerce City
CM3	Adams City High School	39.82736, -104.90193	2.9	E. 72 nd Ave. & Quebec Pkwy, Commerce City
CM4	Adams City Middle School	39.82893, -104.93499	1.9	Birch St. & E. 72 nd Ave., Commerce City
CM5	Central Elementary School	39.81365, -104.92191	1.7	Holly St. & E. 64 th Ave., Commerce City
CM6	Focus Points Family Resource Center	39.78436, -104.95663	1.4	Columbine St. & 48 th Ave., Denver
CM7	Kearney Middle School	39.80888, -104.91545	1.7	E 62 nd Ave. & Kearney St., Commerce City
CM8	Monroe	39.81560, -104.94503	0.85	Monroe St. & E 64 th Ave., Denver
CM9 ¹	Riverside Cemetery	39.78936, -104.96308	1.7	N Brighton Blvd. & Brighton Blvd., Commerce City
CM10	Alsup Elementary School	39.820268, -104.936616	1.2	East 68 th Ave. & Birch St., Commerce City

2.2 Continuous Monitoring

There were ten compounds that were continuously monitored during Q4 of 2025. Six of these compounds (SO₂, NO₂, H₂S, CO, tVOCs, and PM_{2.5}) were initially measured using a network of sensors that were installed at 10 locations across the CCND neighborhood in 2021 and utilized the Sensit RAMP sensors to assess the air concentrations of these compounds as well as meteorological conditions. Sensit RAMP sensors are continuous monitoring instruments that provide near real-time air quality information in the CCND area. Starting on January 1, 2025, Onterris installed the Ambilabs DETECT system with FEM research-grade (Federal Equivalent Method ‘FEM’ equivalent) instruments at CM1, CM2, CM6, CM7, and CM10, followed by the installation at CM8 in April 2025, to comply with new Colorado legislation (HB 24-1338) and Suncor’s Title V permit requirements. The FEM grade sensors have lower limits of detection,

¹ On March 13, 2025, the CM9 monitoring station was moved from the 48th and Race location (39.78455, -104.96264) to the Riverside Cemetery (39.78936, -104.96308). CM9 was relocated after the new owner of the Monroe facility—where the sensor had been installed on the building roof—raised safety and security concerns. The new site, Riverside Cemetery, is located relatively close to the original location, has no known local interference sources, and is easily accessible to the Onterris field team.

providing increased accuracy in the reporting of lower values for four of the compounds (H₂S, NO₂, SO₂, and PM_{2.5}). Details about the DETECT system instruments are described below. Each sensor is solar powered and transmits data to the data platform via Long Term Evolution (LTE) cell technology. The ranges of detection, measurements collected, and measurement frequencies are found in Table 2.

As of January 1, 2025, the Ambilabs DETECT system is also able to measure the concentration of four additional compounds: benzene, toluene, ethylbenzene, and toluene (BTEX compounds) as required by the House Bill 24-1338 and Suncor’s Title V permit requirements. A summary of the CCND air monitoring technology, including the ranges of detection, is provided in Table 2.

Table 2 CCND Air Monitoring Technology

Parameter ^a	CAS Number	Sensit RAMP Range of Detection	Ambilabs DETECT Range of Detection	Detection Interval
Chemical Parameters				
SO ₂	7446-09-5	50 – 1,000 ppb	0.4 – 20,000 ppb	1 minute (Sensit) or 1 minute for 10 minutes intervals (DETECT)
H ₂ S	7783-06-4	10 – 1,000 ppb	0.4 – 10,000 ppb	1 minute (Sensit) or 1 minute for 10 minutes intervals (DETECT)
Benzene	71-43-2	ND	2 – 80 ppb	10 minutes
Toluene	108-88-3	ND	2 – 80 ppb	10 minutes
Ethylbenzene	100-41-4	ND	2 – 200 ppb	10 minutes
Xylene	1330-20-7	ND	2 – 1,000 ppb	10 minutes
NO ₂	10102-44-0	20 – 250 ppb	1 – 10,000 ppb	1 minute
CO	630-08-0	0.05 – 20 ppm	ND	1 minute
Total VOC	--	0.010 – 3 ppm	ND	1 minute
PM _{2.5}	--	1 – 1,000 µg/m ³	0.1 – 10,000 µg/m ³	1 minute
Meteorological Parameters				
Wind Direction	--	NA	ND	1 minute
Wind Speed	--	NA	ND	1 minute
Relative Humidity	--	NA	ND	1 minute
Barometric Pressure	--	NA	ND	1 minute
Temperature	--	NA	ND	1 minute

^a All analytes; NA: not assessed; ND: not detected

The principles of operation for these two sets of sensors are different: the Sensit RAMP instruments monitor the ambient air by allowing it to passively enter each sensor’s exterior housing via small holes and pass over the surface of the sensor, while the FEM research grade instruments use a DETECT system that monitors air by utilizing three instruments: an absorption measurement instrument, a UV analyzer, and a particulate matter measurement instrument.

The FEM research grade instruments use a DETECT system equipped with a 2BTech Model 405, a Teledyne T640, and a Teledyne T101. The Model 405 provides selective direct measurement of NO₂ by absorbance at 405 nm. The Model T101 analyzer uses the proven UV fluorescence principle to measure H₂S and SO₂ at levels commonly required for ambient air monitoring. The Model T101 is equipped with an internally mounted catalytic converter set at 315°C to convert H₂S to SO₂. The Model T101 operates in a switching mode in which it measures H₂S and SO₂ every 10 minutes. During each 10-minute cycle, the analyzer reports one minute data points for H₂S or SO₂, respectively. The Teledyne API Model T640 is a real-time, FEM, continuous particulate matter mass monitor that uses scattered light spectrometry for measurement of PM_{2.5}.

The BTEX compounds were monitored using the Pyxis GC by Pollution Analytical Equipment. The main components of the device are a pre-concentrator, a gas chromatography micro-electro-mechanical (GC MEMS) column and a photoionization (PID) detector. The GC MEMS column does not require a carrier gas cylinder to operate. The time resolution for the analysis of each sample is 10 minutes. During the 10-minute analysis cycle, the device analyzes the previously collected sample, while simultaneously collecting a new air sample. The analysis begins by collecting a composite air sample using a high-volume transport fan, where a small slipstream of air sample is collected for analysis; this sample is collected on the sample modulator or pre-concentrator for analysis. This sample is transferred to the GC column (GC) for separation. As the chemicals elute from the column, they are detected by a PID sensor.

The Sensit RAMP utilizes a PID to measure VOCs. In other words, it utilizes a lamp that produces photons that carry enough energy to break molecules into ions. The PID responds to molecules that have an ionization energy at or below the energy of the lamp; the PID used on this project employs a 10.6 electron-volt lamp. The produced ions then generate an electrical current that is measured as the output of the detector. PIDs can be susceptible to drift with ambient temperature and humidity variations. The PIDs used in this program mitigate the humidity issue by having a hydrophobic filter installed between the lamp and the ambient air. This deters water molecules from entering the ion-producing chamber and absorbing radiation. The PIDs are also heated slightly above ambient temperature to improve the stability of the detector. Meanwhile, the Sensit RAMP also uses electrochemical sensors to measure the concentration of CO. The oxidation and reduction reactions generate the positive or negative current flow through the external circuit. It is then quantified by amperometry. All of these components sit inside a sensor housing along with a liquid electrolyte that is specific to the compound of interest.

Meteorological conditions are also collected by the Sensit RAMP, including temperature and ambient relative humidity data.

While data are collected in 1-minute or 10-minute intervals depending on the sensor, background concentrations may interfere with the sensors and make it difficult to effectively quantify concentrations of specific compounds. To combat this, the raw data were exported as five-minute averages and then were aggregated to the 1-hour or 24-hour (H₂S and benzene only) level by calculating rolling averages for all compounds except PM_{2.5}. For PM_{2.5}, block averages were calculated at 1-hour and 24-hour intervals.

In addition, data recovery percentages were calculated. This is done by dividing the number of data points collected by the expected number of data points. For example, if a data point is expected every five minutes, 12 data points would be expected over a one-hour period. If only 11 data points were received, the data recovery for that hour would be 92%.

The data presented here are intended to be used for informational purposes only and are not intended to be used for official NAAQS or other compliance determinations given that the calculations for NAAQS as required by the USEPA or for other compliance standards are not performed in this report. The sensors' detection limits and accuracy can be found in Table 2. State regulatory compliance data can be found on the CDPHE air quality website at <https://www.colorado.gov/airquality>. All sampling and quality assurance procedures were performed by Onterris.

2.3 Assessment of Real-Time Air Monitoring Trends

This report does not include a formal risk assessment or calculation of exposure metrics. Rather, 1-hour and 24-hour averages are plotted over time to review trends in air concentrations of various compounds in the CCND communities. To understand how these values generally compare to established reference levels, health scientists from Onterris Response and Recovery, LLC, provided the United States Environmental Protection Agency (USEPA) Acute Exposure Guideline Levels (AEGLs), USEPA National Ambient Air Quality Standards (NAAQS), and the Agency for Toxic Substances and Disease Registry (ATSDR) acute minimum risk levels (MRLs) for comparison purposes only.

The available 1-hour AEGL values are utilized as the data are presented as 1-hour average concentrations. AEGL values are levels at which different acute adverse health effects may be anticipated to occur. However, a concentration above an AEGL-1 value does not necessarily mean that health effects will occur. According to USEPA, "AEGL-1 represents exposure levels that could produce mild and progressively increasing but transient and non-disabling odor, taste, and sensory irritation or certain asymptomatic, non-sensory effects. With increasing airborne concentration above each AEGL, there is a progressive increase in the likelihood of occurrence and the severity of effects described for each corresponding AEGL [i.e., AEGL-2 or AEGL-3]."² The AEGL-1 60-minute (i.e., 1-hour) value, if available for the applicable chemical, was used for comparison purposes because it is more precautionary (than AEGL-2 or AEGL-3) as the AEGL-1 level reflects protecting against acute health effects that are reversible upon cessation of exposure. For CO, the 1-hour AEGL-2 value was the only available comparison value and thus, was used. AEGLs are typically used in emergency situations for single exposure events; however, the presented data are compared against the AEGL values to evaluate trends in air monitoring data and are not intended to represent a risk assessment.

Four of the compounds (CO, NO₂, SO₂, and PM_{2.5}) are criteria air pollutants that are regulated under the USEPA NAAQS. To determine NAAQS compliance, specific calculations must be performed

² <https://www.epa.gov/aegl/about-acute-exposure-guideline-levels-aegls>

according to a defined set of equations.³ The values in this report are not formal calculations of concentration comparisons for NAAQS as required by USEPA; therefore, 1-hour values above the relevant NAAQS are not intended to represent NAAQS compliance or risk for adverse health effects. The purpose of these values, as presented here, is to demonstrate trends in criteria pollutant levels in the CCND communities, and NAAQS values are used to help contextualize those trends.

Finally, the ATSDR acute health-based reference levels (i.e., acute MRLs, which represent one day to two weeks of continuous exposure) were also used. The ATSDR MRLs are levels below which continuous exposure is likely to be without risk of developing adverse health effects, even in sensitive sub-populations.⁴ However, a concentration above an MRL does not necessarily mean that adverse health effects will occur.

For general comparison purposes only, these reference levels are shown against the 1-hour and 24-hour analyte concentration averages, with the comparable averaging interval presented (Table 3).

3.0 Results

3.1 Results Summary

Continuous air monitoring sensors were operating at ten locations across the CCND neighborhoods from October 1 – December 31, 2025.⁵ The data from this reporting period were aggregated into 1-hour and 24-hour block averages for PM_{2.5}, and 1-hour or 24-hour rolling averages for all other compounds. The results from the continuous air monitoring program are found below in Table 3 and in Figures 2 – 14. While the target percent raw data recovery (%RDR) or data completeness is 95% per the QAPP, the real-time air monitoring network-wide %RDR was >93%. Instrument malfunction, communication issues, downtime while performing quality assurance procedures, and theft are all possible explanations for a %RDR below 100%. In addition, extreme humidity, temperature, and adverse weather conditions can impact the ability of the sensors to effectively detect compounds. The results of the air monitoring conducted in Q4 of 2025 indicate the following:

- For all compounds except benzene (24-hour rolling average), rolling and/or block average concentrations fell below their respective health-based RLs.
- The 24-hour rolling average concentrations of benzene was above the ATSDR Acute MRL (9 ppb) at CM1 on October 2 (9.34 – 9.80 ppb) and October 14 (9.26 – 13.32 ppb), 2025. Notably,

³ <https://www.epa.gov/criteria-air-pollutants/naaqs-table>

⁴ <https://www.cdc.gov/tsp/mrls/mrlslisting.aspx>

⁵ No valid H₂S and SO₂ measurements were collected at CM6 during Q4 2025 given that the monitor at this location failed weekly QC tests. Additionally, CM7 Ambilabs DETECT BTEX monitor failed calibration check on September 26, 2025, resulting in invalid data from October 1 – 5, 2025. Therefore, no valid BTEX measurements were collected at CM7 during this period. Finally, CM10 Ambilabs DETECT BTEX monitor experienced power outages and failed calibration on October 9, 2025, October 13 – 15, 2025, and October 18 – 26, 2025. Therefore, no valid BTEX measurements were collected at CM10 during these periods. The PID in the CM10 BTEX monitor was replaced December 12, 2025, resulting in a lowered baseline through the end of the quarter.

the CM1 BTEX sensor showed an elevated baseline and kept failing the bump test for all BTEX compounds beginning on September 29, 2025. Therefore, it was determined that the BTEX sensor had a malfunctioning PID source, which resulted in an elevated baseline and could potentially be the reason for these higher benzene concentrations. The system was serviced and the PID source was replaced on October 16, 2025, after which the baseline decreased.

- No valid H₂S and SO₂ measurements were collected at CM6 during Q4 2025 given that the monitor at this location failed weekly QC tests. The team determined that a faulty UV lamp caused the instrument baseline to gradually increase each week and then decrease following the weekly calibration sequence, resulting in invalid measurements. The UV lamp was replaced during Q1 2026.
- During a total of four trigger events, the tVOC 1-minute measurements exceeded the 1 ppm threshold and triggered the collection of four canister samples. The results of these triggered canister analyses will be available in a separate report at <https://www.ccnd-air.com/>.

Table 3 CCND Monitors Results Summary⁶

Compound	Range of 5-min Data Recovery	Averaging Type	Rolling/Block Average Range ^a	NAAQS	Health-Based Reference Level (Source)
FEM Sensors (CM1, CM2, CM6, CM7, and CM10)					
Benzene	80.4 – 97.2%	1-hour rolling	<2 – 13.3 ppb	NA	52,000 ppb ^e (USEPA 1-hour AEGL-1)
		24-hour rolling	<2 – 12.5 ppb	NA	9 ppb (ATSDR Acute MRL)
Ethylbenzene	80.4 – 97.2%	1-hour rolling	<2 – 8.1 ppb	NA	33,000 ppb ^e (USEPA 1-hour AEGL-1)
Toluene	80.4 – 97.2%	1-hour rolling	<2 – 16.5 ppb	NA	67,000 ppb ^e (USEPA 1-hour AEGL-1)
Xylenes	80.4 – 97.2%	1-hour rolling	<2 – 33.1 ppb	NA	130,000 ppb ^e (USEPA 1-hour AEGL-1)
All Sites (CM1 – CM10)					
CO	95.3 – 99.4%	1-hour rolling	<0.05 – 2.0 ppm	35 ppm ^f	83 ppm (USEPA 1-hour AEGL-2)
tVOC	95.3 – 99.4%	1-hour rolling	<0.01 – 0.67 ppm	NA	NA
H ₂ S	90.2 – 99.2%	1-hour rolling	<10 – 75.1 ppb	NA	510 ppb (USEPA 1-hour AEGL-1)
		24-hour rolling	<10 – 17.2 ppb	NA	70 ppb (ATSDR Acute MRL)
NO ₂	90.8 – 99.2%	1-hour rolling	<20 – 81.2 ppb	100 ppb ^b	500 ppb (USEPA 1-hour AEGL-1)
PM _{2.5} ^g	92.0 – 99.5%	1-hour block	<1 – 119.6 µg/m ³	NA	NA
		24-hour block	<1 – 21.0 µg/m ³	35 µg/m ³ ^c	NA
SO ₂	90.5 – 99.2%	1-hour rolling	<50 – 17.8 ppb	75 ppb ^d	200 ppb (USEPA 1-hour AEGL-1)

^a“<” indicates a value was below the instrument’s limit of detection; ^b Annual 98th percentile of 1-hour daily maximum concentrations, averaged over 3 years; ^c Annual 98th percentile of 24-hour daily average concentrations, averaged over 3 years; ^d Annual 99th percentile of 1-hour daily maximum concentrations, averaged over 3 years; ^e The upper detection limits for the real-time instruments monitoring the CCND area are 80 ppb for benzene and toluene, 200 ppb for ethylbenzene, and 1,000 ppb for xylene; therefore, the 1-hour AEGL-1 values are not used as a comparison for these compounds, given that these reference levels are outside the detection range of the real-time instruments; ^f 1-hour; not to be exceeded more than once per year. ^g Data recovery rate for PM_{2.5} was calculated based on the number of valid 1-hour block averages. NA = Not available

⁶ No valid H₂S and SO₂ measurements were collected at CM6 during Q4 2025 given that the monitor at this location failed weekly QC tests; thus, CM6 for H₂S and SO₂ was excluded from this table.

Figure 2 CCND Community Monitoring Carbon Monoxide (CO) 1-Hour Rolling Average Data

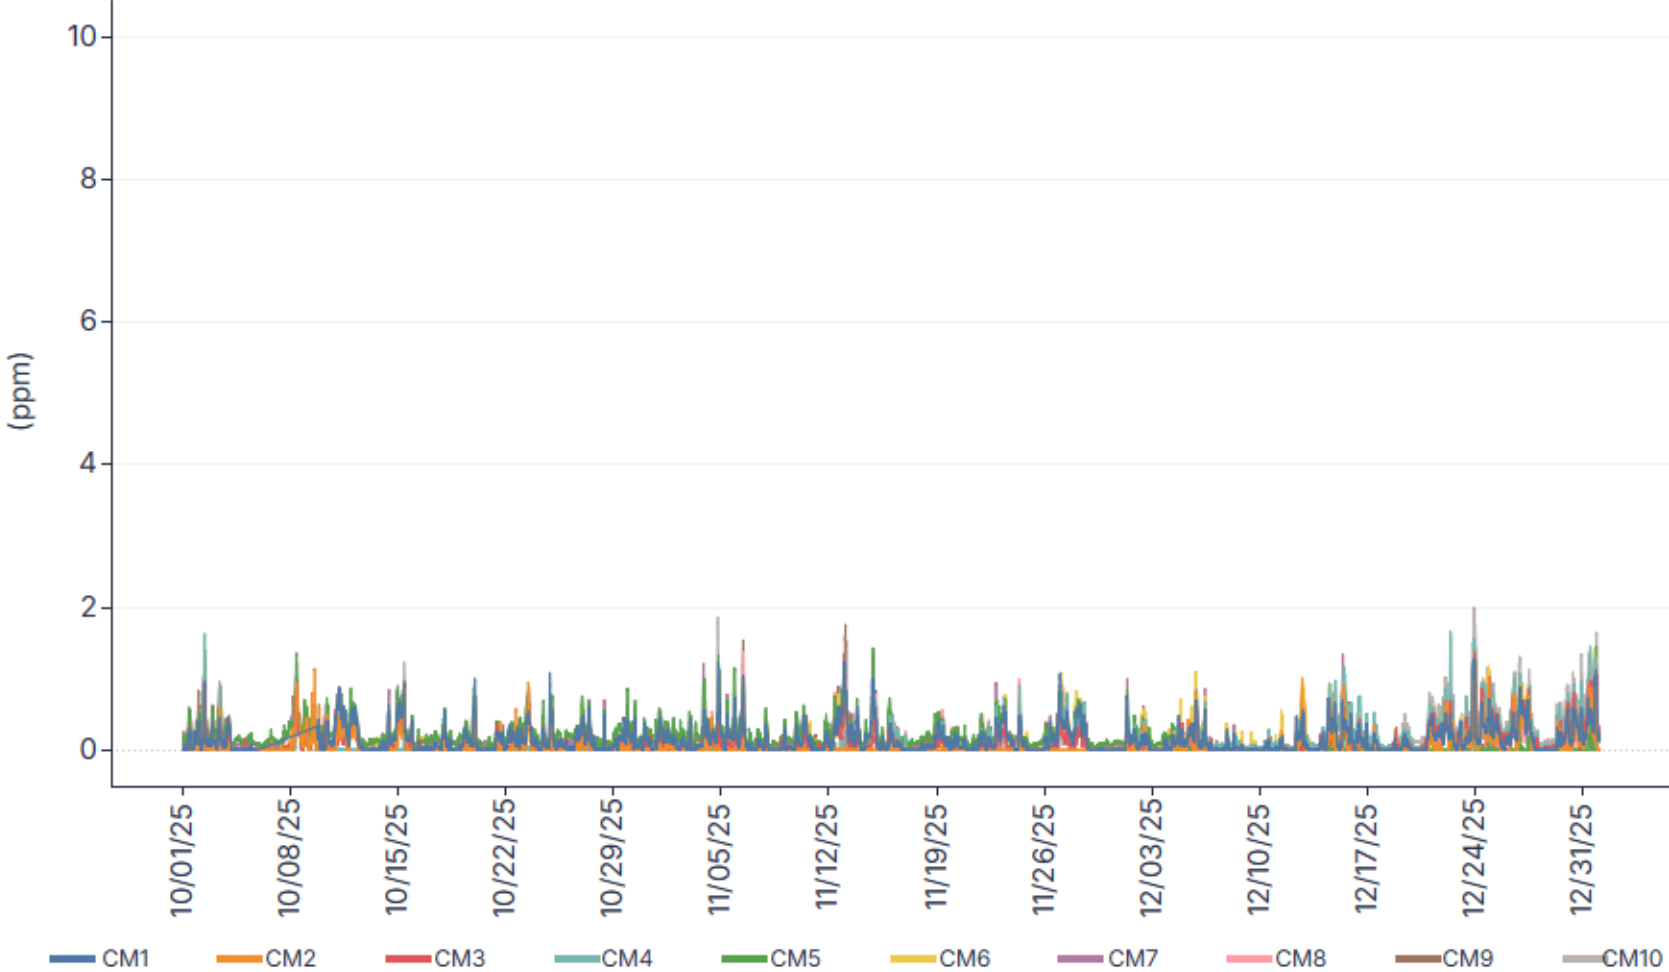


Figure 3 CCND Community Monitoring Nitrogen Dioxide (NO₂) 1-Hour Rolling Average Data



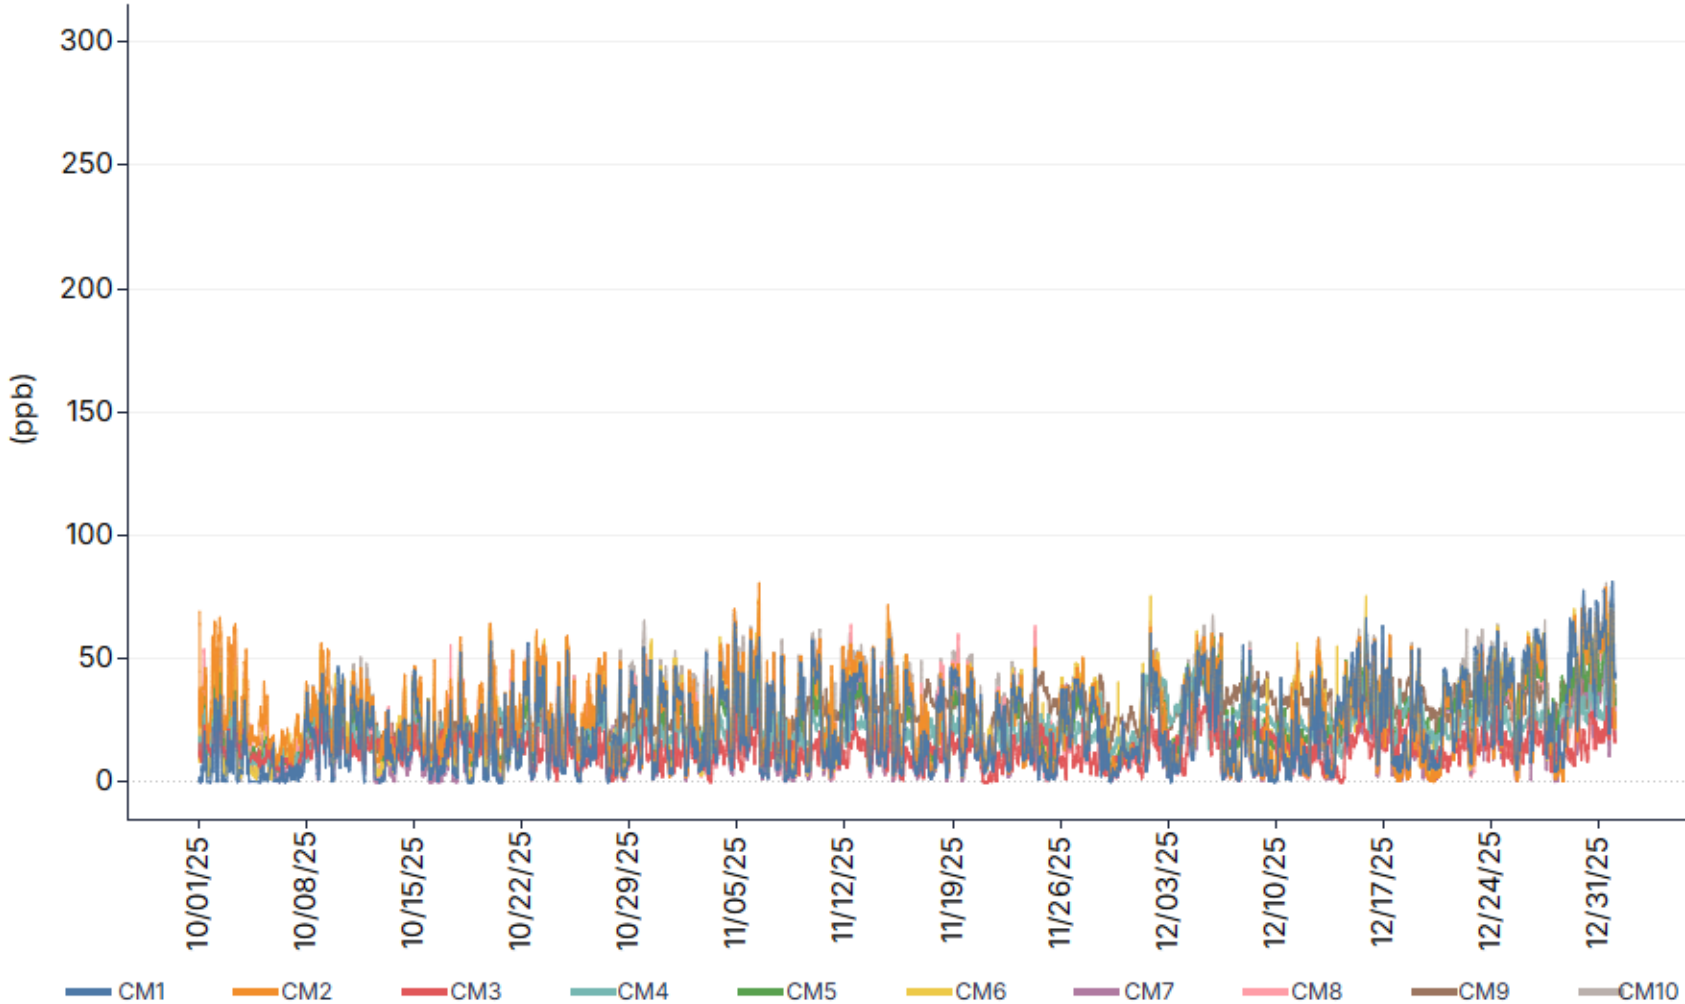


Figure 4 CCND Community Monitoring Sulfur Dioxide (SO₂) 1-Hour Rolling Average Data⁷

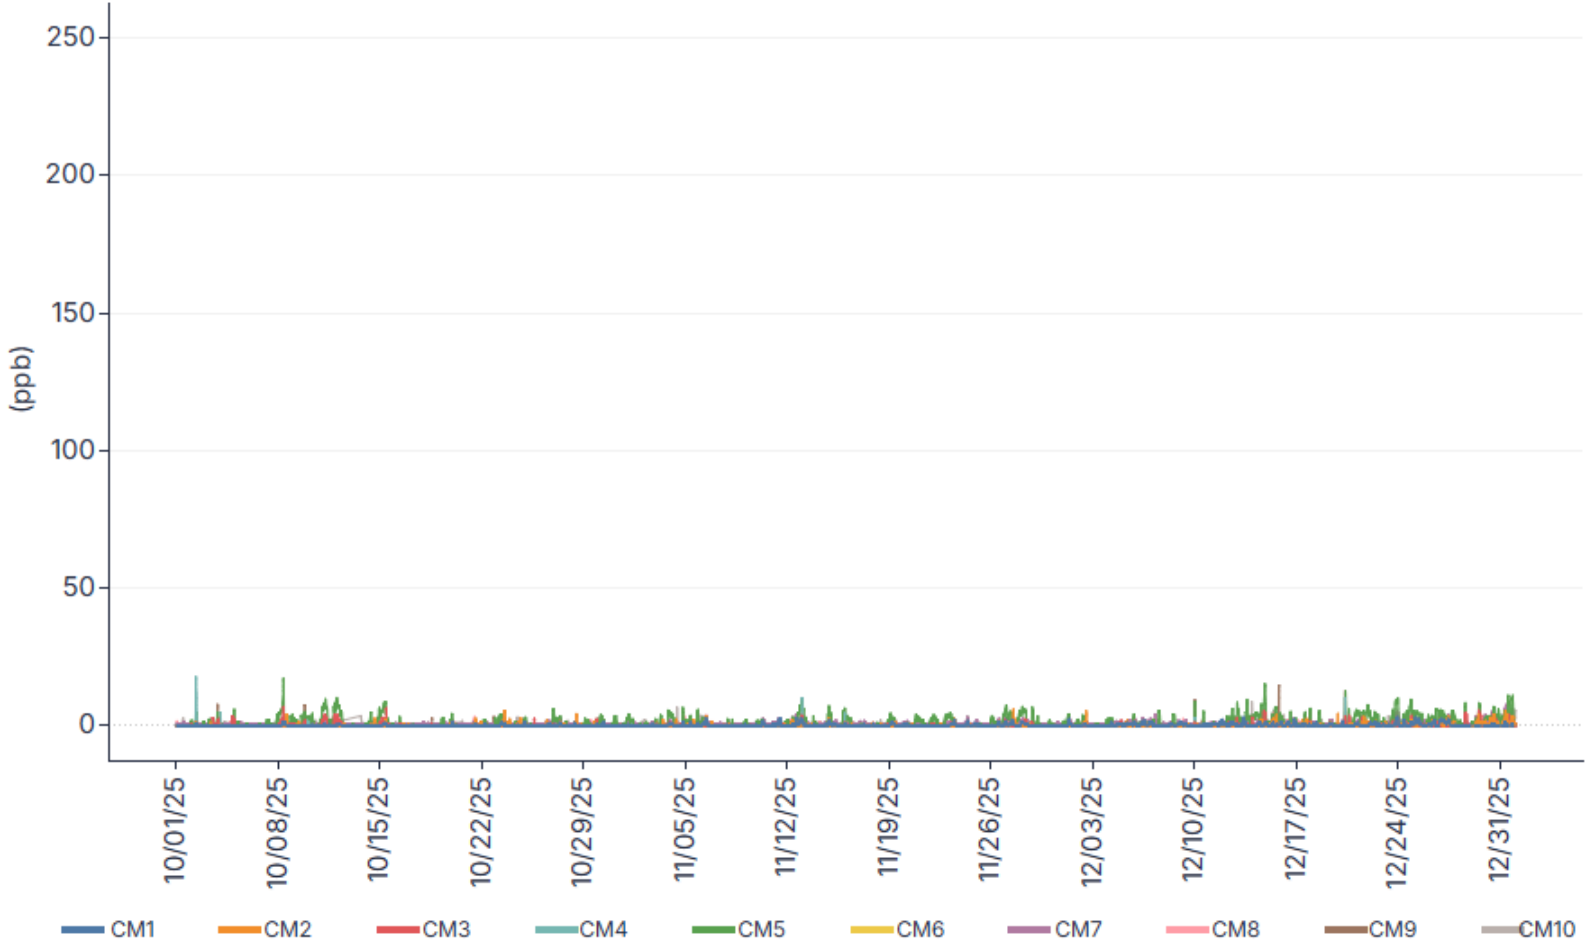


⁷ No valid SO₂ measurements were collected at CM6 during this quarter given that the monitor at this location failed weekly QC tests.

Figure 5 CCND Community Monitoring Hydrogen Sulfide (H₂S) 1-Hour Rolling Average Data⁸

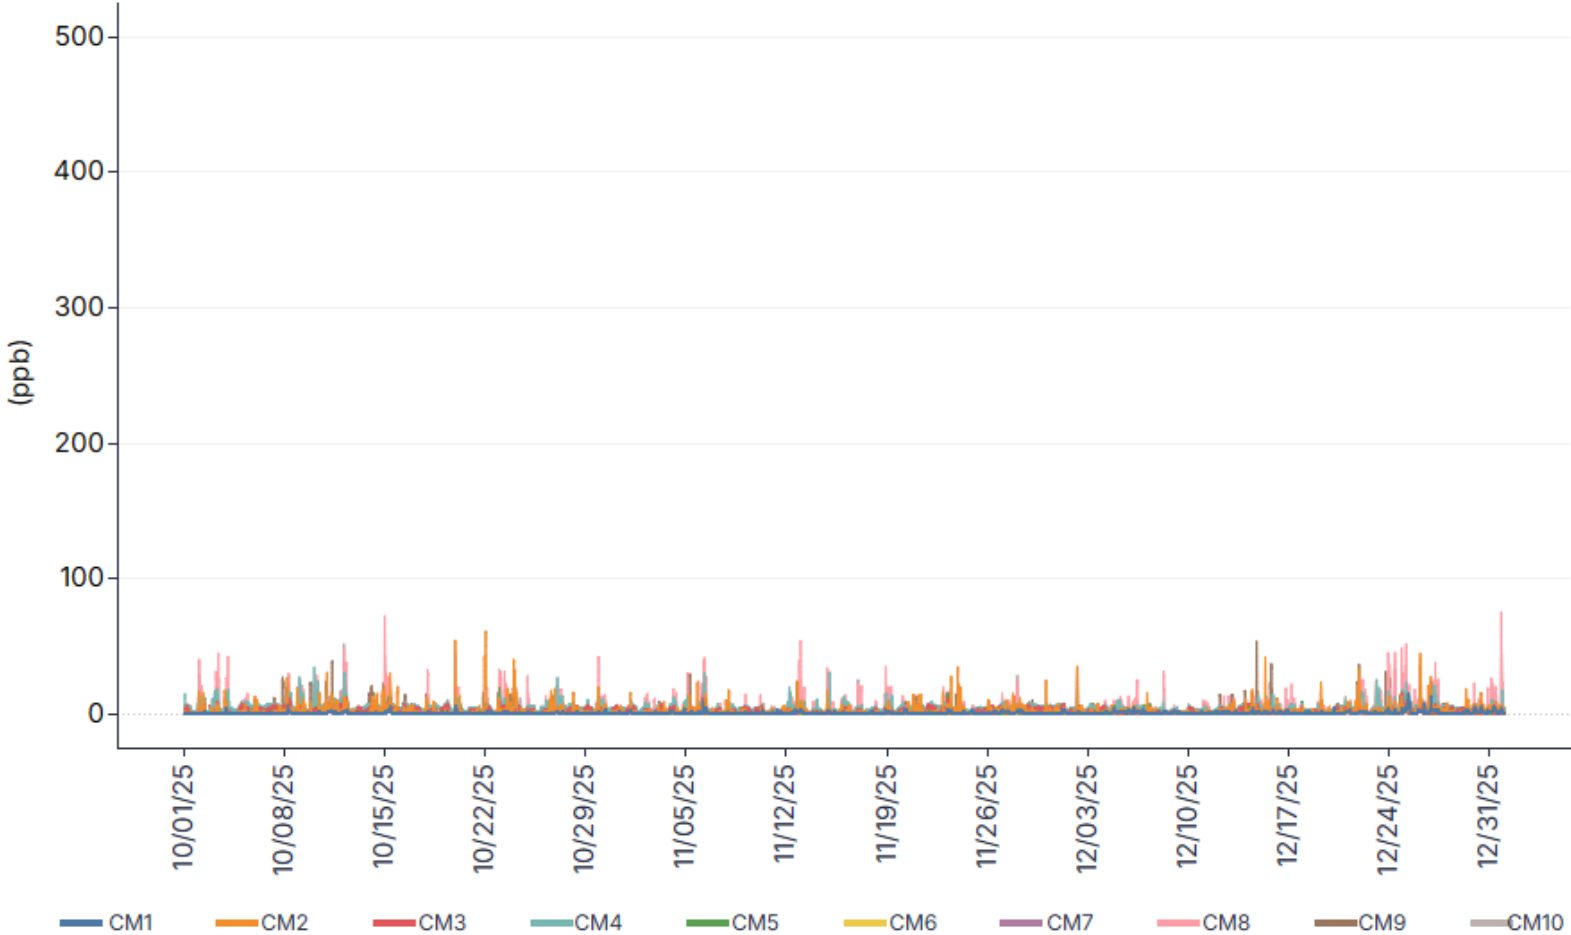

⁸ No valid H₂S measurements were collected at CM6 during this quarter given that the monitor at this location failed weekly QC tests.

Figure 6 CCND Community Monitoring Hydrogen Sulfide (H₂S) 24-Hour Rolling Average Data⁹

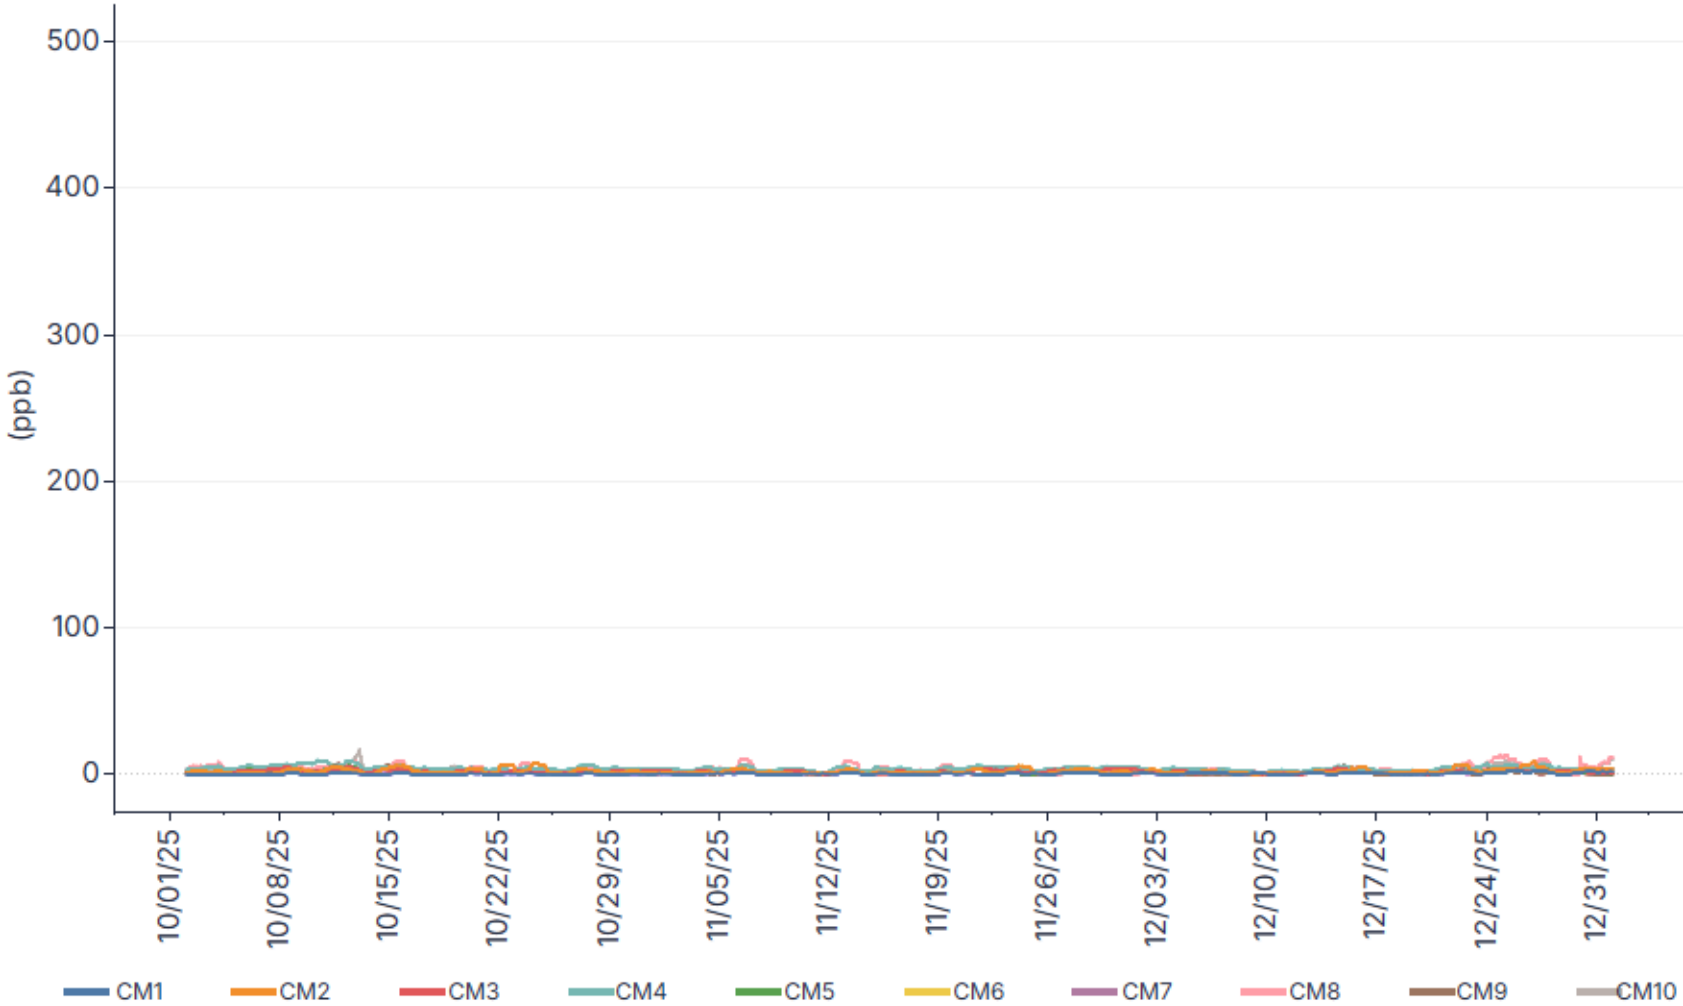

⁹ No valid H₂S measurements were collected at CM6 during this quarter given that the monitor at this location failed weekly QC tests.

Figure 7 CCND Community Monitoring PM_{2.5} 1-Hour Block Average Data

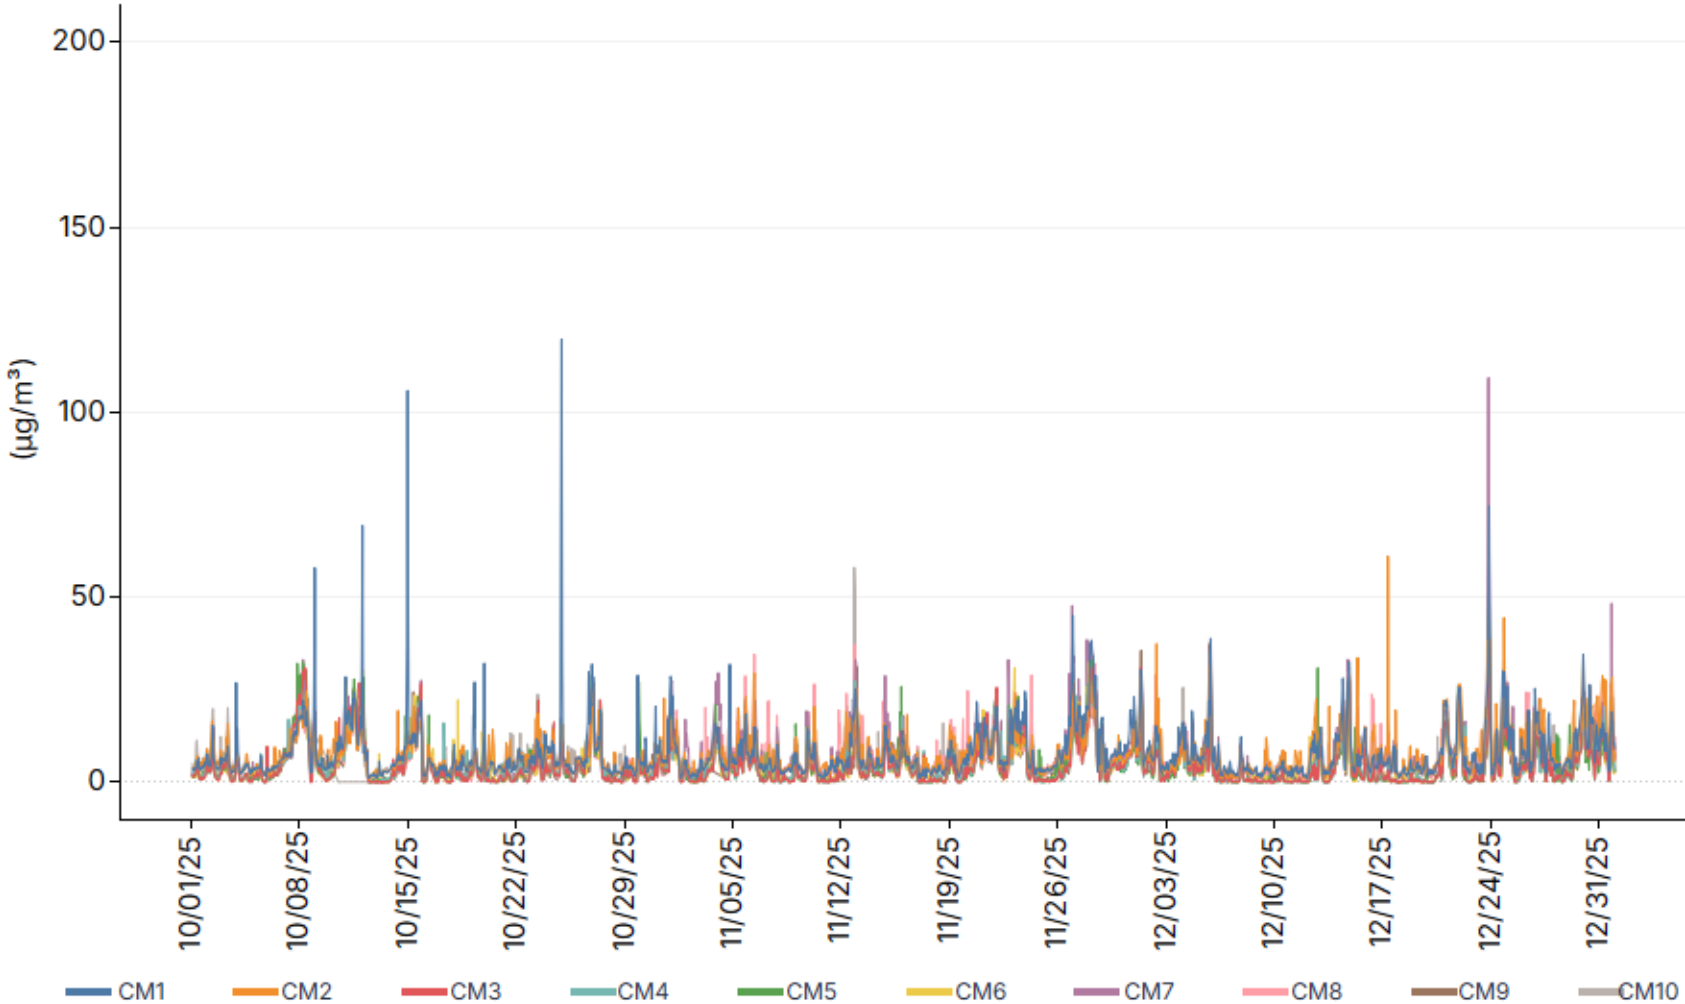


Figure 8 CCND Community Monitoring PM_{2.5} 24-Hour Block Average Data

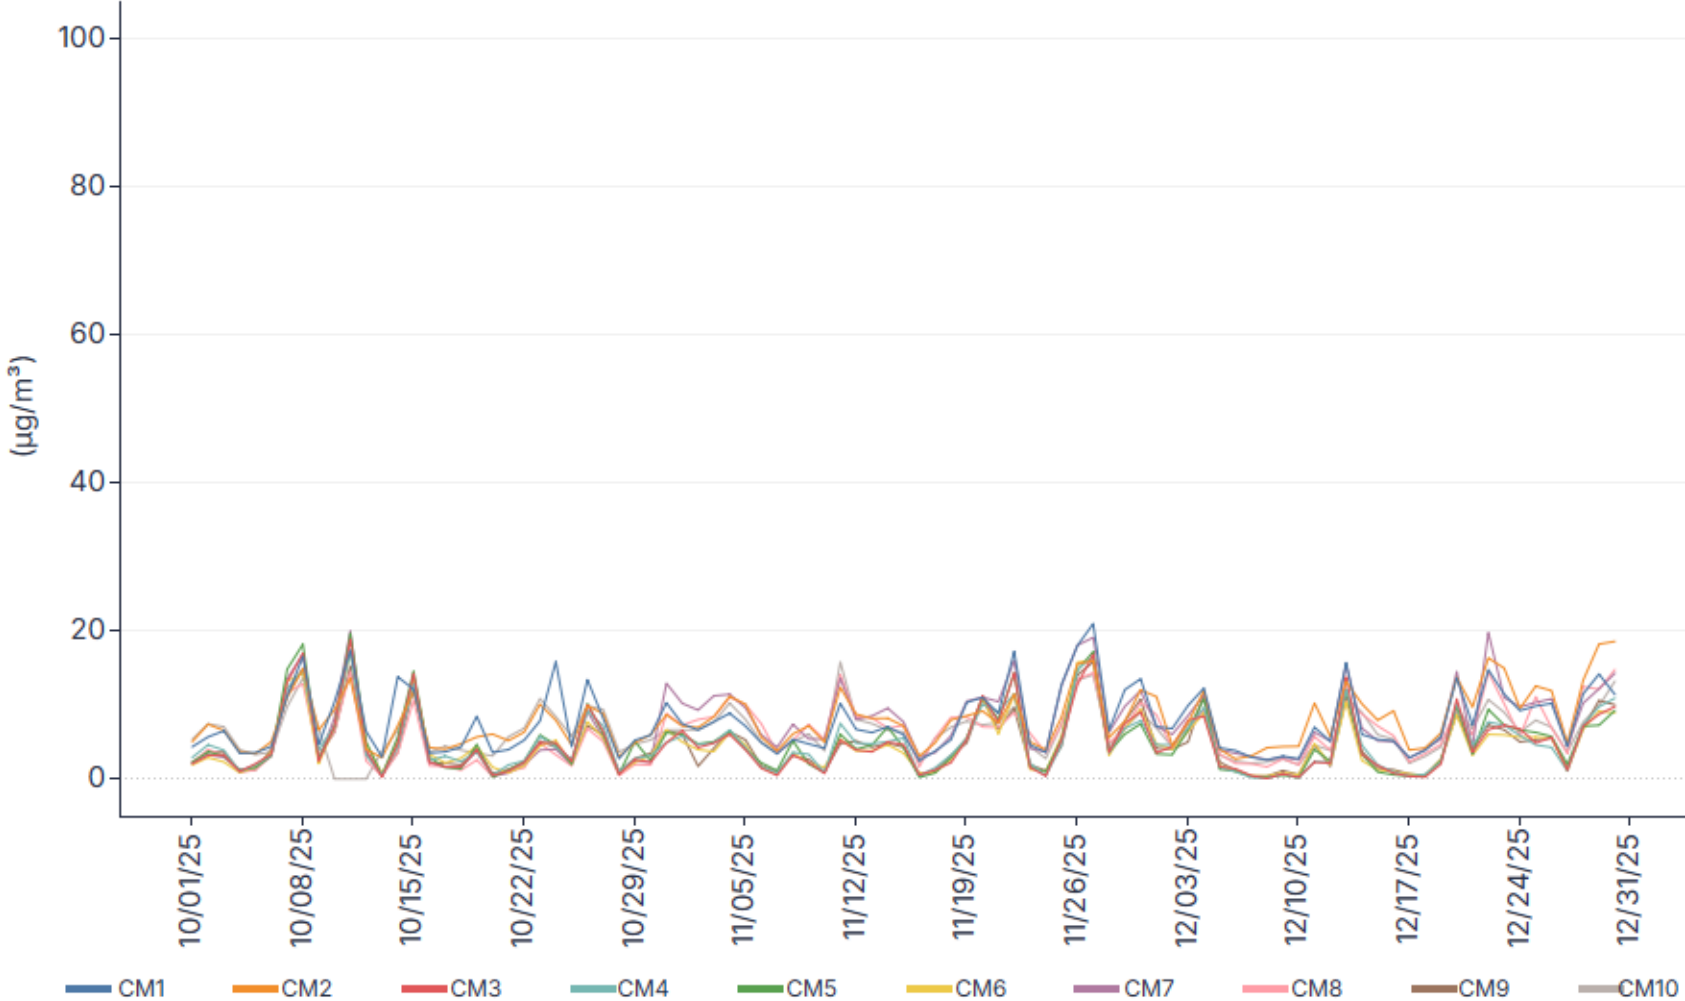


Figure 9 CCND Community Monitoring tVOC 1-Hour Rolling Average Data



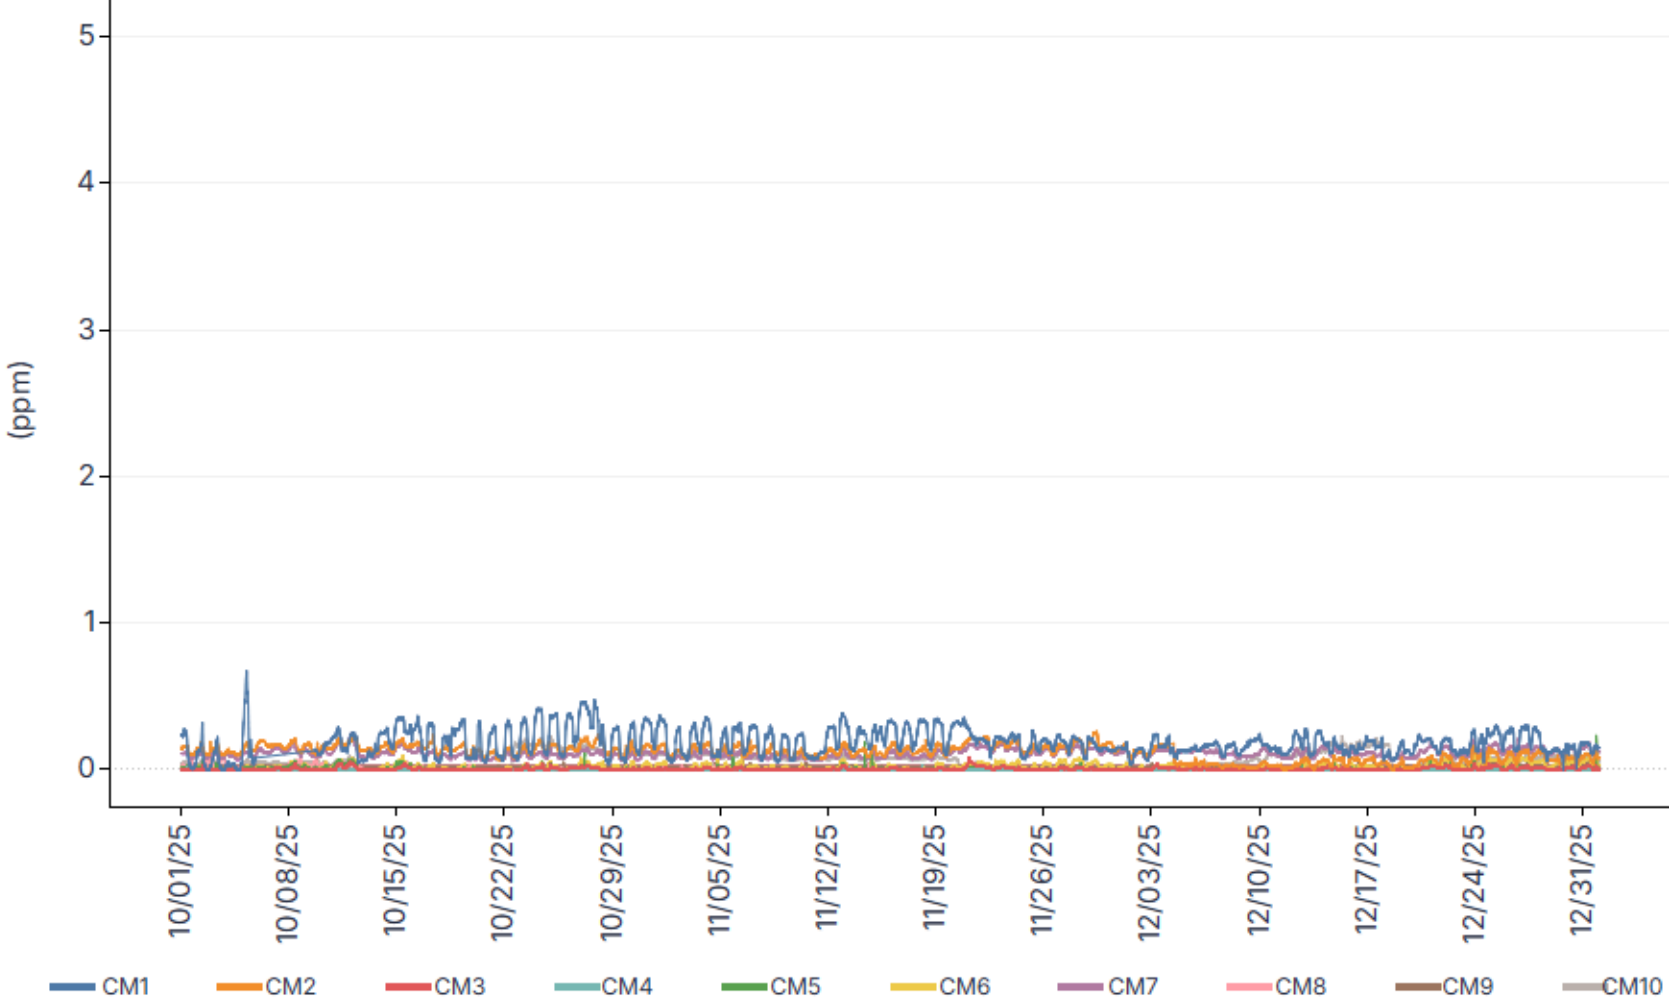


Figure 10 CCND Community Monitoring Benzene 1-Hour Rolling Average Data¹⁰

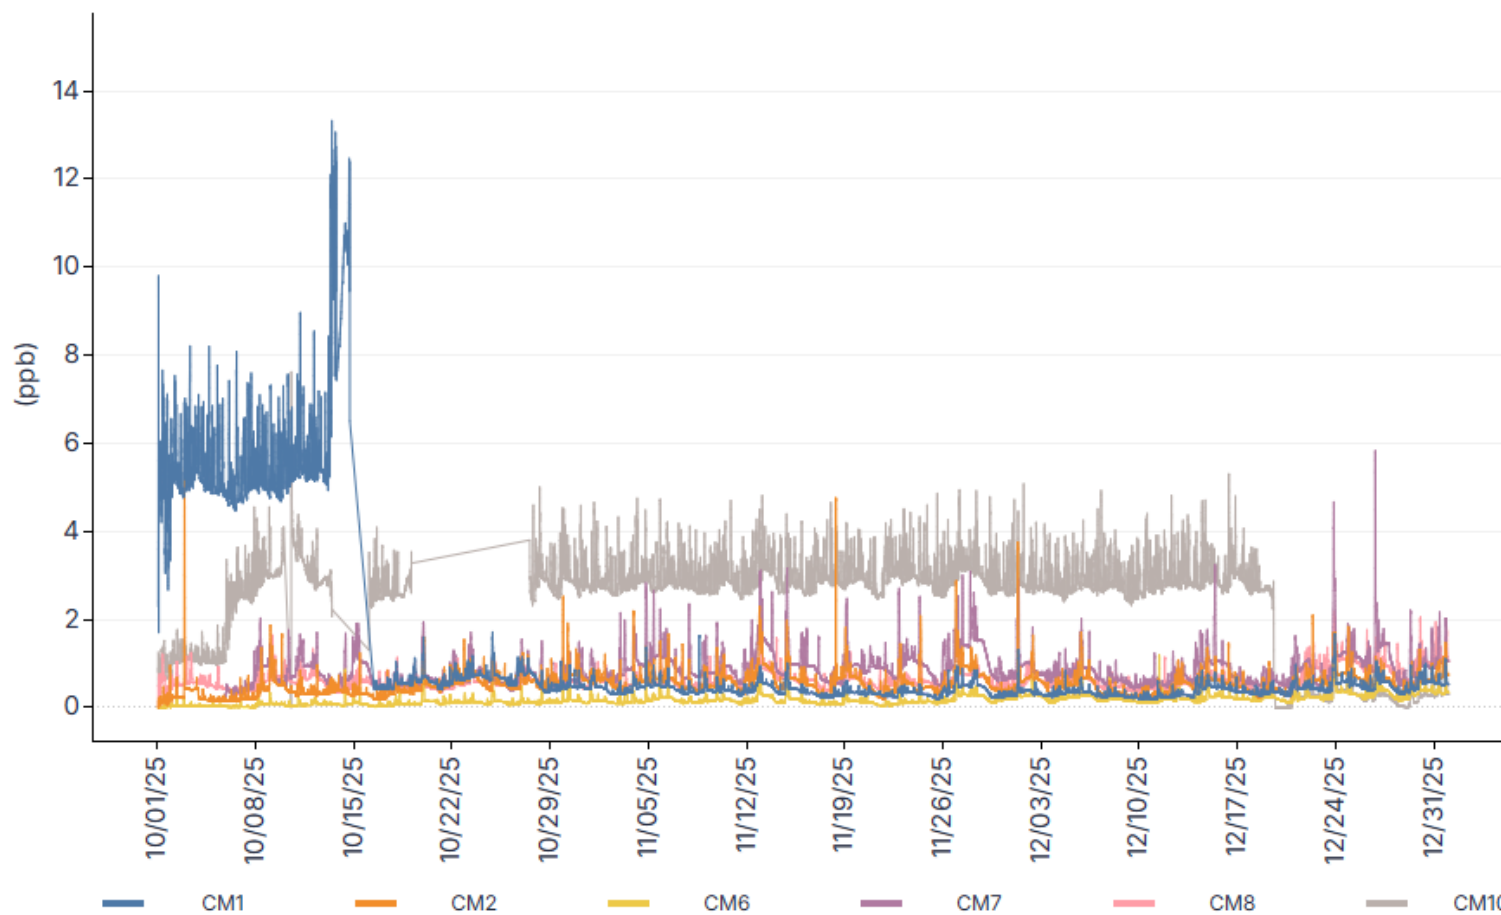


¹⁰ CM10 Ambilabs DETECT BTEX monitor experienced power outages and failed calibration on October 9, 2025, October 13 – 15, 2025, and October 18 – 26, 2025. Additionally, CM7 Ambilabs DETECT BTEX monitor failed calibration check on September 26, 2025, resulting in invalid data from October 1 – 5, 2025. Therefore, no valid BTEX measurements were collected at these locations during these periods. The PID in the CM10 BTEX monitor was replaced December 12, 2025, resulting in a lowered baseline through the end of the quarter.

Figure 11 CCND Community Monitoring Benzene 24-Hour Rolling Average Data¹¹

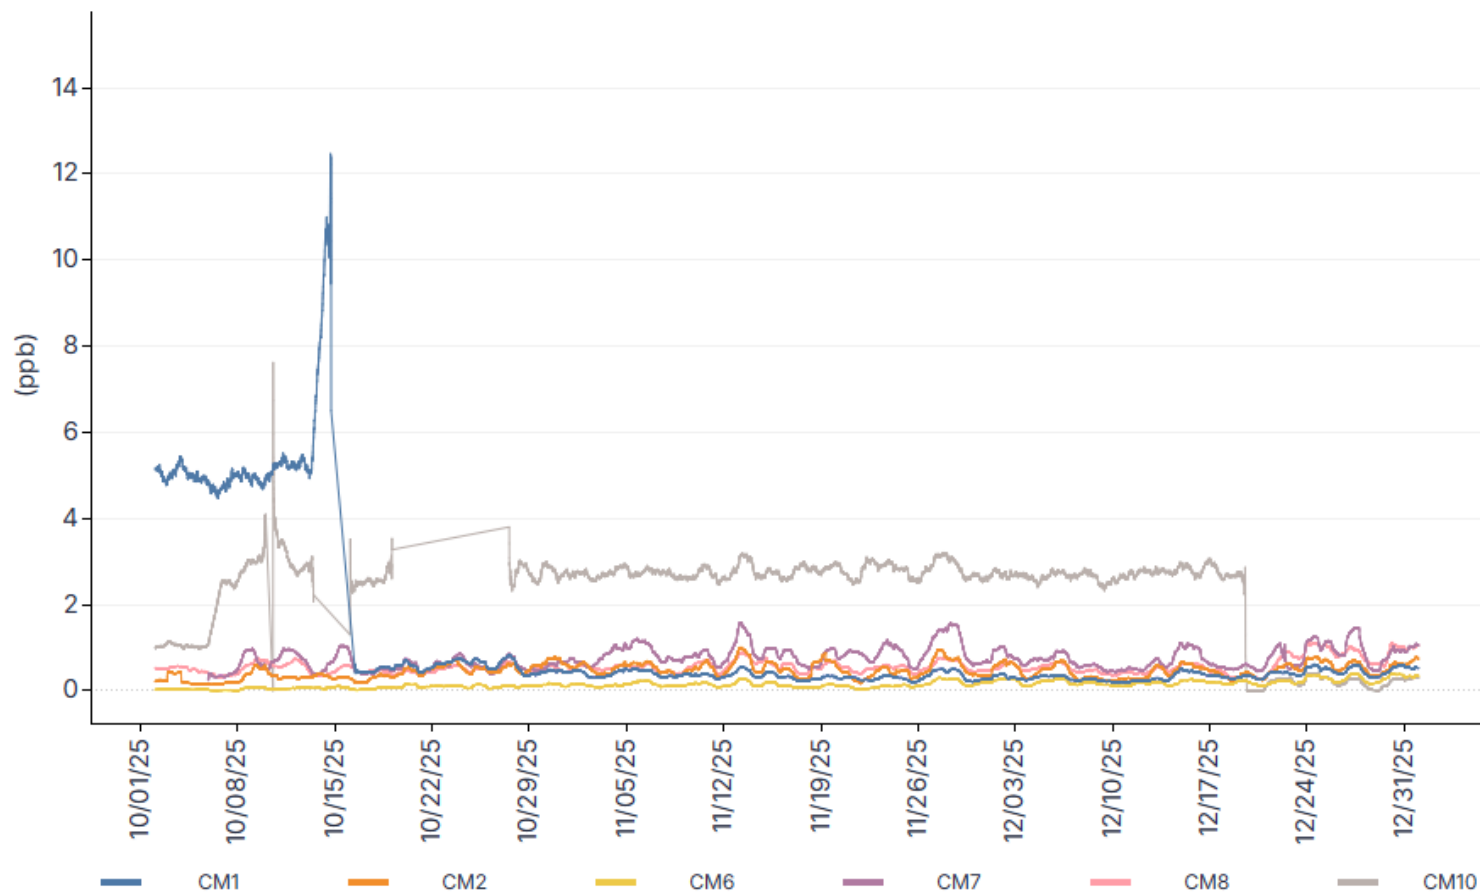


¹¹ CM10 Ambilabs DETECT BTEX monitor experienced power outages and failed calibration on October 9, 2025, October 13 – 15, 2025, and October 18 – 26, 2025. Additionally, CM7 Ambilabs DETECT BTEX monitor failed calibration check on September 26, 2025, resulting in invalid data from October 1 – 5, 2025. Therefore, no valid BTEX measurements were collected at these locations during these periods. The PID in the CM10 BTEX monitor was replaced December 12, 2025, resulting in a lowered baseline through the end of the quarter.

Figure 12 CCND Community Monitoring Ethylbenzene 1-Hour Rolling Average Data¹²

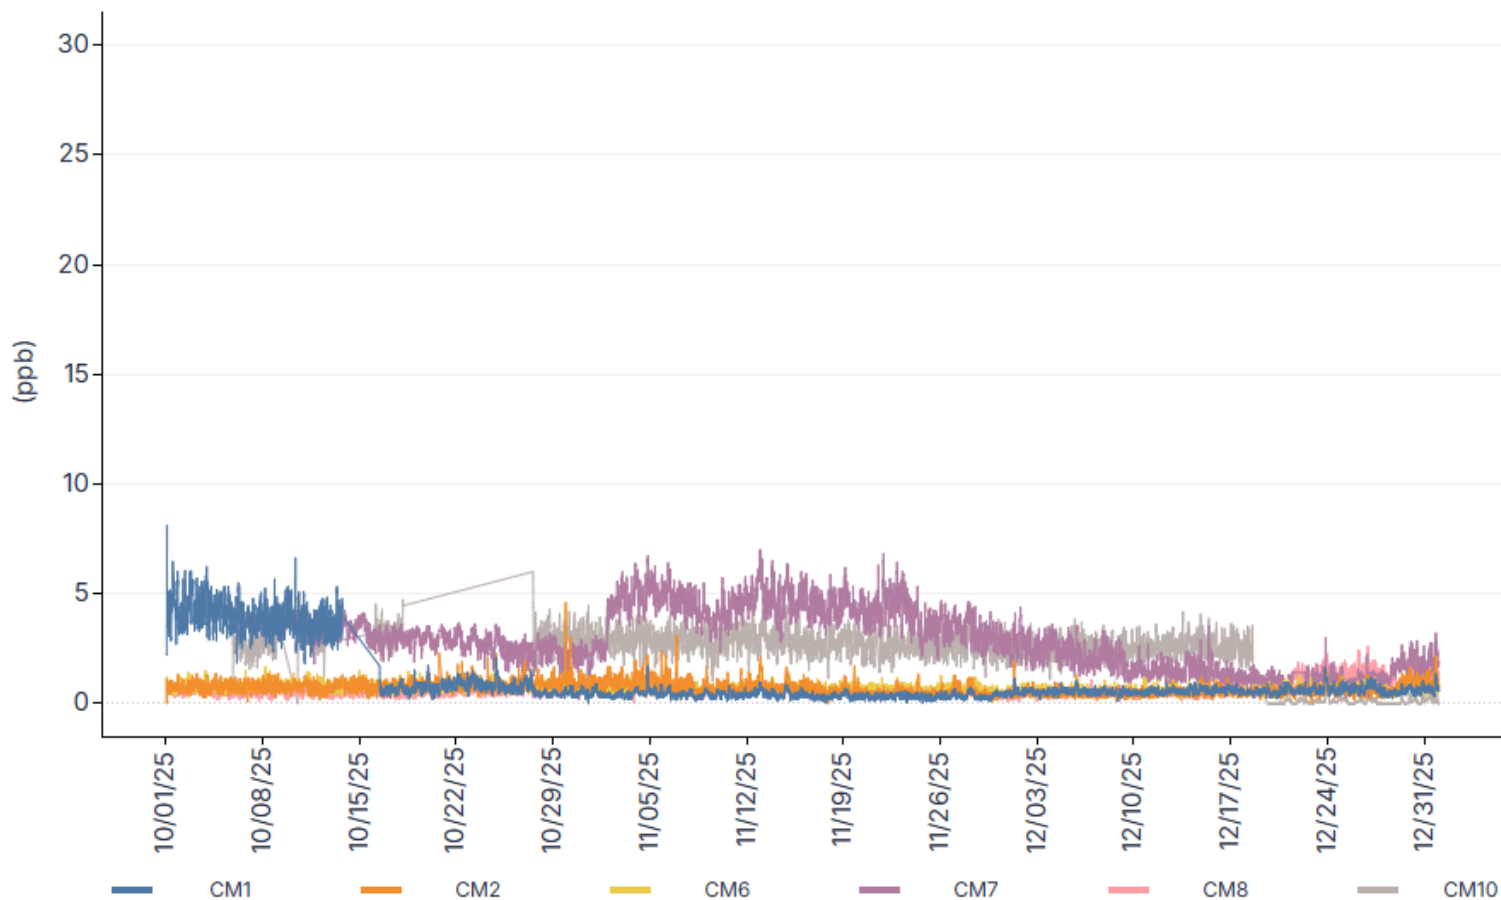


¹² CM10 Ambilabs DETECT BTEX monitor experienced power outages and failed calibration on October 9, 2025, October 13 – 15, 2025, and October 18 – 26, 2025. Additionally, CM7 Ambilabs DETECT BTEX monitor failed calibration check on September 26, 2025, resulting in invalid data from October 1 – 5, 2025. Therefore, no valid BTEX measurements were collected at these locations during these periods. The PID in the CM10 BTEX monitor was replaced December 12, 2025, resulting in a lowered baseline through the end of the quarter.

Figure 13 CCND Community Monitoring 1-Hour Rolling Average Toluene Data¹³

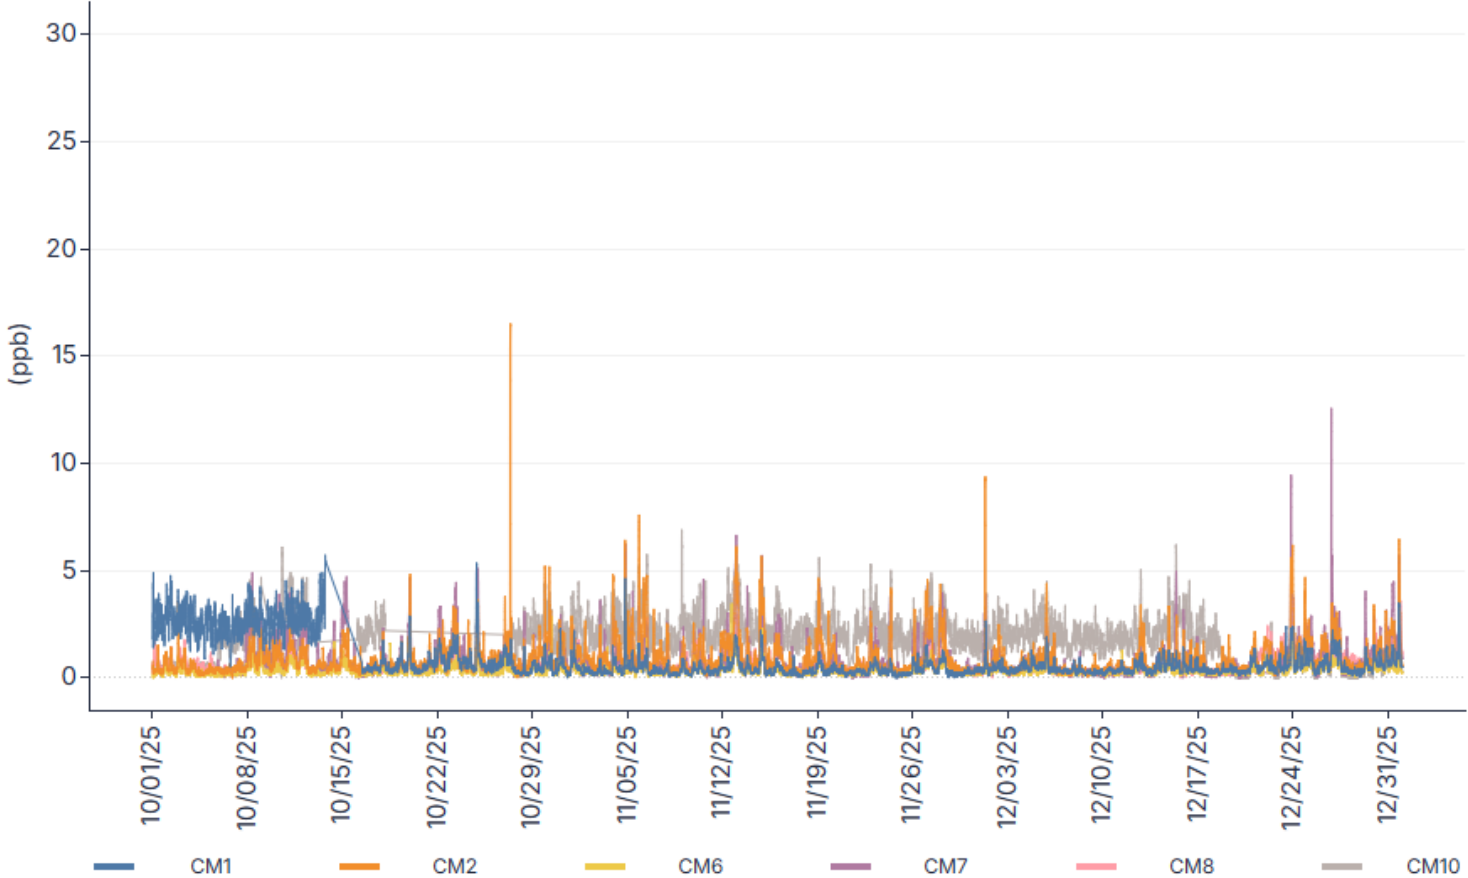

¹³ CM10 Ambilabs DETECT BTEX monitor experienced power outages and failed calibration on October 9, 2025, October 13 – 15, 2025, and October 18 – 26, 2025. Additionally, CM7 Ambilabs DETECT BTEX monitor failed calibration check on September 26, 2025, resulting in invalid data from October 1 – 5, 2025. Therefore, no valid BTEX measurements were collected at these locations during these periods. The PID in the CM10 BTEX monitor was replaced December 12, 2025, resulting in a lowered baseline through the end of the quarter.

Figure 14 CCND Community Monitoring 1-Hour Rolling Average Xylene Data¹⁴

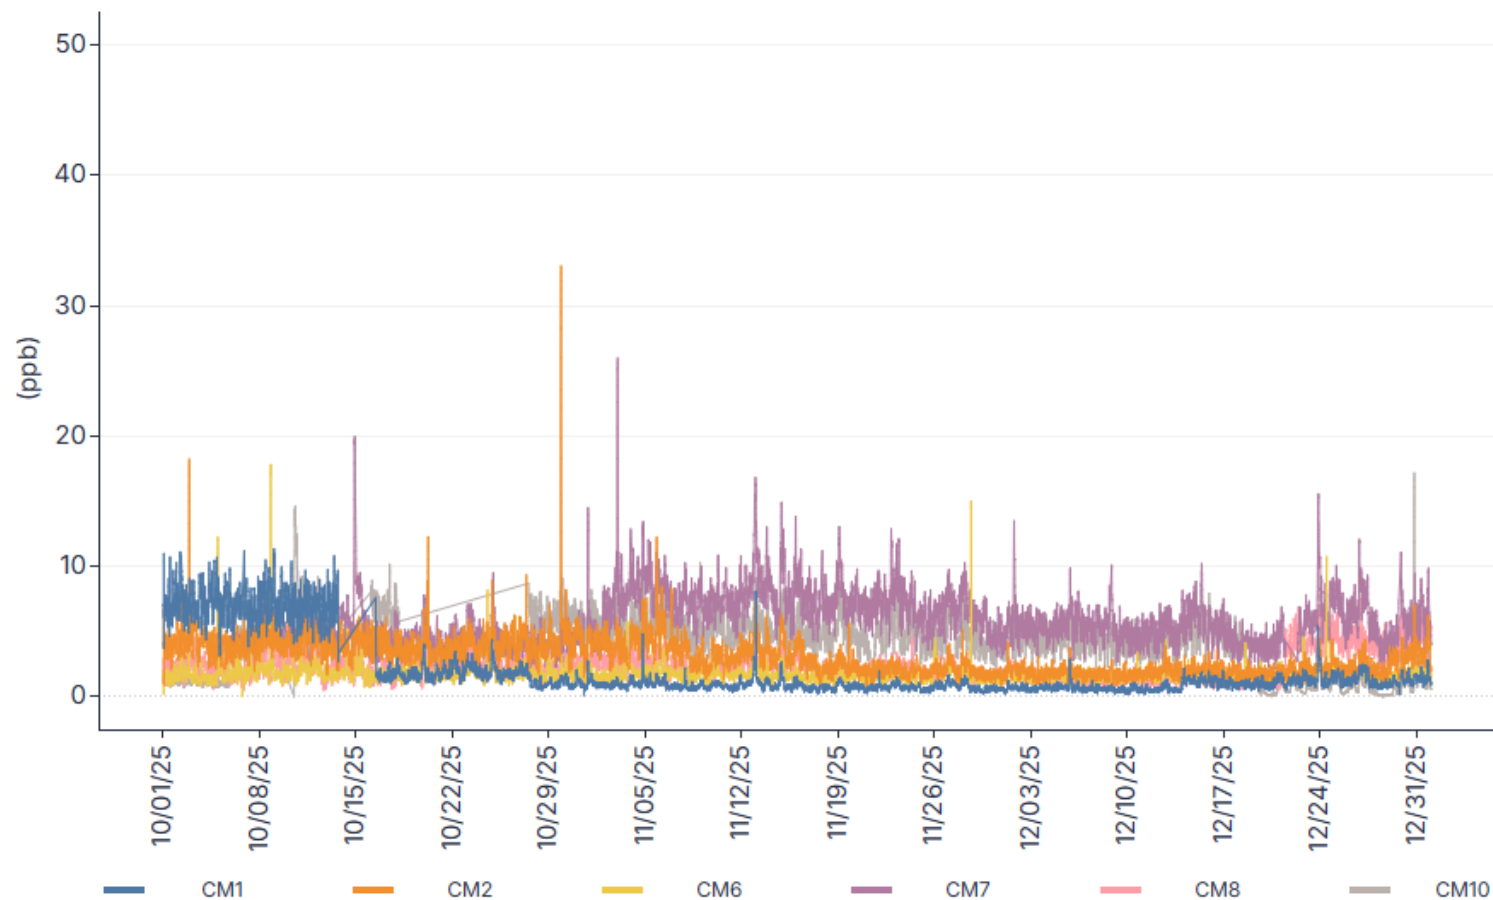


¹⁴ CM10 Ambilabs DETECT BTEX monitor experienced power outages and failed calibration on October 9, 2025, October 13 – 15, 2025, and October 18 – 26, 2025. Additionally, CM7 Ambilabs DETECT BTEX monitor failed calibration check on September 26, 2025, resulting in invalid data from October 1 – 5, 2025. Therefore, no valid BTEX measurements were collected at these locations during these periods. The PID in the CM10 BTEX monitor was replaced December 12, 2025, resulting in a lowered baseline through the end of the quarter.

4.0 Program changes

No program changes are reported for this quarter.

Prepared by:



Antonios Tasoglou, PhD, PMP
Emergency Technology Manager
Onterris Air Quality Services, LLC

Appendix A Calibration and QA/QC Data

Date	Location	Parameter	Precision (error)	Span (error)	Zero (absolute value)
10/6/2025	CM1	H2S	1.60%	0.80%	0.5
10/6/2025	CM1	NO	3.60%	4.30%	1.1
10/6/2025	CM1	NO2	1.90%	29.80%	4.9
10/6/2025	CM1	SO2	5.70%	7.60%	0.5
10/6/2025	CM1	Benzene	N/A	33.50%	3.2
10/6/2025	CM1	Toluene	N/A	31.00%	1.7
10/6/2025	CM1	Ethylbenzene	N/A	20.80%	4.9
10/6/2025	CM1	Xylenes	N/A	10.60%	6
10/13/2025	CM1	H2S	0.40%	0.30%	0.4
10/13/2025	CM1	NO	3.20%	1.00%	0.4
10/13/2025	CM1	NO2	8.90%	0.20%	2.1
10/13/2025	CM1	SO2	5.10%	5.50%	0.3
10/13/2025	CM1	Benzene	N/A	16.30%	4.4
10/13/2025	CM1	Toluene	N/A	23.00%	3.5
10/13/2025	CM1	Ethylbenzene	N/A	33.80%	4.1
10/13/2025	CM1	Xylenes	N/A	25.20%	3.4
10/20/2025	CM1	H2S	0.90%	0.10%	0.4
10/20/2025	CM1	NO	2.00%	2.60%	0.5
10/20/2025	CM1	NO2	9.50%	0.60%	2.9
10/20/2025	CM1	SO2	5.20%	6.20%	0.4
10/20/2025	CM1	Benzene	N/A	58.30%	0.3
10/20/2025	CM1	Toluene	N/A	87.80%	0.4
10/20/2025	CM1	Ethylbenzene	N/A	87.80%	0.8
10/20/2025	CM1	Xylenes	N/A	84.50%	1.9
10/27/2025	CM1	H2S	0.40%	0.60%	0.4
10/27/2025	CM1	NO	2.00%	3.90%	0
10/27/2025	CM1	NO2	3.90%	1.90%	0
10/27/2025	CM1	SO2	5.90%	6.60%	0.6
10/27/2025	CM1	Benzene	N/A	17.50%	0.1
10/27/2025	CM1	Toluene	N/A	19.30%	0.2
10/27/2025	CM1	Ethylbenzene	N/A	22.00%	0.3
10/27/2025	CM1	Xylenes	N/A	24.40%	1
11/3/2025	CM1	H2S	1.20%	1.10%	0.4
11/3/2025	CM1	NO	2.70%	4.30%	0.3
11/3/2025	CM1	NO2	4.30%	3.80%	0.5
11/3/2025	CM1	SO2	7.50%	7.80%	0.5
11/3/2025	CM1	Benzene	N/A	13.80%	0.2
11/3/2025	CM1	Toluene	N/A	14.80%	0.1
11/3/2025	CM1	Ethylbenzene	N/A	14.80%	0.6
11/3/2025	CM1	Xylenes	N/A	13.80%	0.9
11/10/2025	CM1	H2S	1.50%	2.80%	0.3

11/10/2025	CM1	NO	2.80%	4.30%	0.3
11/10/2025	CM1	NO2	3.70%	5.00%	0
11/10/2025	CM1	SO2	5.60%	6.80%	0.1
11/10/2025	CM1	Benzene	N/A	14.50%	0.2
11/10/2025	CM1	Toluene	N/A	15.00%	0
11/10/2025	CM1	Ethylbenzene	N/A	12.50%	0.7
11/10/2025	CM1	Xylenes	N/A	10.60%	0.7
11/17/2025	CM1	H2S	0.30%	1.10%	0.1
11/17/2025	CM1	NO	1.70%	2.60%	0
11/17/2025	CM1	NO2	2.30%	3.20%	4.4
11/17/2025	CM1	SO2	6.50%	8.20%	0.4
11/17/2025	CM1	Benzene	N/A	23.00%	0.4
11/17/2025	CM1	Toluene	N/A	29.00%	0.1
11/17/2025	CM1	Ethylbenzene	N/A	29.00%	0.1
11/17/2025	CM1	Xylenes	N/A	28.40%	0.8
11/24/2025	CM1	H2S	0.30%	0.20%	0.2
11/24/2025	CM1	NO	2.30%	4.10%	0.9
11/24/2025	CM1	NO2	2.90%	2.90%	1.9
11/24/2025	CM1	SO2	7.90%	8.60%	0.2
11/24/2025	CM1	Benzene	N/A	26.80%	0.1
11/24/2025	CM1	Toluene	N/A	30.50%	0
11/24/2025	CM1	Ethylbenzene	N/A	33.50%	0.2
11/24/2025	CM1	Xylenes	N/A	29.60%	0.6
12/1/2025	CM1	H2S	0.80%	0.10%	0.3
12/1/2025	CM1	NO	1.10%	4.10%	0.3
12/1/2025	CM1	NO2	1.20%	5.20%	1.9
12/1/2025	CM1	SO2	6.50%	6.00%	0
12/1/2025	CM1	Benzene	N/A	25.80%	0.2
12/1/2025	CM1	Toluene	N/A	4.00%	0.1
12/1/2025	CM1	Ethylbenzene	N/A	5.50%	0.3
12/1/2025	CM1	Xylenes	N/A	26.40%	1.2
12/8/2025	CM1	H2S	0.30%	1.00%	0.4
12/8/2025	CM1	NO	2.90%	0.50%	0.7
12/8/2025	CM1	NO2	6.30%	3.80%	4.4
12/8/2025	CM1	SO2	6.00%	5.30%	0.4
12/8/2025	CM1	Benzene	N/A	31.00%	0.2
12/8/2025	CM1	Toluene	N/A	3.50%	0.1
12/8/2025	CM1	Ethylbenzene	N/A	0.30%	0.4
12/8/2025	CM1	Xylenes	N/A	30.10%	1.1
12/15/2025	CM1	H2S	1.10%	0.90%	0.2
12/15/2025	CM1	NO	1.50%	4.00%	0.2
12/15/2025	CM1	NO2	0.70%	5.70%	1.4
12/15/2025	CM1	SO2	5.70%	6.40%	0.3
12/15/2025	CM1	Benzene	N/A	2.00%	0.1
12/15/2025	CM1	Toluene	N/A	1.50%	0.3
12/15/2025	CM1	Ethylbenzene	N/A	2.30%	0.4

12/15/2025	CM1	Xylenes	N/A	4.00%	0.8
12/22/2025	CM1	H2S	10.70%	25.10%	0.3
12/22/2025	CM1	NO	8.50%	22.40%	1
12/22/2025	CM1	NO2	2.30%	18.80%	0.4
12/22/2025	CM1	SO2	3.70%	17.50%	0.2
12/22/2025	CM1	Benzene	N/A	N/A	0.1
12/22/2025	CM1	Toluene	N/A	N/A	0.2
12/22/2025	CM1	Ethylbenzene	N/A	N/A	0.5
12/22/2025	CM1	Xylenes	N/A	N/A	1.4
12/29/2025	CM1	H2S	23.50%	5.70%	0.2
12/29/2025	CM1	NO	17.50%	4.50%	0.2
12/29/2025	CM1	NO2	25.20%	0.30%	7.3
12/29/2025	CM1	SO2	20.30%	8.60%	2.2
12/29/2025	CM1	Benzene	N/A	N/A	0.1
12/29/2025	CM1	Toluene	N/A	N/A	0.3
12/29/2025	CM1	Ethylbenzene	N/A	N/A	0.8
12/29/2025	CM1	Xylenes	N/A	N/A	0.7

RBC DETECT

Date	Location	Parameter	Precision (error)	Span (error)	Zero (absolute value)
10/6/2025	CM2	H2S	4.80%	2.90%	1
10/6/2025	CM2	NO	3.20%	0.50%	1
10/6/2025	CM2	NO2	1.70%	10.60%	2.7
10/6/2025	CM2	SO2	0.80%	2.50%	1
10/6/2025	CM2	Benzene	N/A	0.30%	0.7
10/6/2025	CM2	Toluene	N/A	3.80%	0.1
10/6/2025	CM2	Ethylbenzene	N/A	2.30%	0.4
10/6/2025	CM2	Xylenes	N/A	1.20%	4.1
10/13/2025	CM2	H2S	5.90%	2.80%	0.1
10/13/2025	CM2	NO	4.00%	2.20%	0.1
10/13/2025	CM2	NO2	4.40%	2.70%	0.2
10/13/2025	CM2	SO2	1.20%	4.00%	1.1
10/13/2025	CM2	Benzene	N/A	12.80%	0.3
10/13/2025	CM2	Toluene	N/A	9.80%	0.2
10/13/2025	CM2	Ethylbenzene	N/A	12.00%	1.1
10/13/2025	CM2	Xylenes	N/A	17.40%	5.5
10/20/2025	CM2	H2S	7.30%	3.20%	0.1
10/20/2025	CM2	NO	25.50%	32.30%	0.4
10/20/2025	CM2	NO2	3.10%	0.20%	4.8
10/20/2025	CM2	SO2	0.80%	0.70%	0.8
10/20/2025	CM2	Benzene	N/A	19.80%	0.3
10/20/2025	CM2	Toluene	N/A	12.80%	0.4

10/20/2025	CM2	Ethylbenzene	N/A	3.00%	2.1
10/20/2025	CM2	Xylenes	N/A	8.50%	2.2
10/27/2025	CM2	H2S	5.50%	3.10%	0.1
10/27/2025	CM2	NO	43.50%	46.90%	0.3
10/27/2025	CM2	NO2	10.90%	0.20%	5.4
10/27/2025	CM2	SO2	2.30%	1.20%	1.2
10/27/2025	CM2	Benzene	N/A	39.30%	0.2
10/27/2025	CM2	Toluene	N/A	27.30%	0.2
10/27/2025	CM2	Ethylbenzene	N/A	17.30%	1.5
10/27/2025	CM2	Xylenes	N/A	19.20%	2.6
11/3/2025	CM2	H2S	6.90%	4.10%	0.4
11/3/2025	CM2	NO	4.70%	0.30%	0
11/3/2025	CM2	NO2	3.10%	4.00%	3.6
11/3/2025	CM2	SO2	0.10%	2.30%	0.7
11/3/2025	CM2	Benzene	N/A	16.30%	0.5
11/3/2025	CM2	Toluene	N/A	49.50%	0
11/3/2025	CM2	Ethylbenzene	N/A	42.50%	0.5
11/3/2025	CM2	Xylenes	N/A	50.20%	1.8
11/10/2025	CM2	H2S	8.10%	4.20%	0.6
11/10/2025	CM2	NO	3.50%	0.00%	0.7
11/10/2025	CM2	NO2	0.70%	3.80%	4.2
11/10/2025	CM2	SO2	4.10%	1.10%	0.8
11/10/2025	CM2	Benzene	N/A	24.50%	0.2
11/10/2025	CM2	Toluene	N/A	18.30%	0.3
11/10/2025	CM2	Ethylbenzene	N/A	32.80%	0.4
11/10/2025	CM2	Xylenes	N/A	37.90%	2.8
11/17/2025	CM2	H2S	6.30%	3.60%	0.4
11/17/2025	CM2	NO	14.40%	18.50%	1.2
11/17/2025	CM2	NO2	2.50%	0.40%	0.9
11/17/2025	CM2	SO2	3.30%	0.30%	1
11/17/2025	CM2	Benzene	N/A	29.80%	0.3
11/17/2025	CM2	Toluene	N/A	17.30%	0
11/17/2025	CM2	Ethylbenzene	N/A	5.00%	0
11/17/2025	CM2	Xylenes	N/A	4.70%	2.2
11/24/2025	CM2	H2S	9.90%	4.10%	0.3
11/24/2025	CM2	NO	17.20%	18.60%	1.7
11/24/2025	CM2	NO2	5.20%	1.90%	1.6
11/24/2025	CM2	SO2	0.00%	0.40%	0
11/24/2025	CM2	Benzene	N/A	25.80%	0.2
11/24/2025	CM2	Toluene	N/A	19.50%	0.2
11/24/2025	CM2	Ethylbenzene	N/A	2.30%	0.4
11/24/2025	CM2	Xylenes	N/A	2.60%	2.4
12/1/2025	CM2	H2S	10.40%	5.80%	0.2
12/1/2025	CM2	NO	0.10%	3.30%	0.3
12/1/2025	CM2	NO2	1.10%	4.10%	0.3
12/1/2025	CM2	SO2	2.70%	0.30%	0.7

12/1/2025	CM2	Benzene	N/A	26.00%	0.6
12/1/2025	CM2	Toluene	N/A	15.30%	0.1
12/1/2025	CM2	Ethylbenzene	N/A	3.50%	0.2
12/1/2025	CM2	Xylenes	N/A	1.90%	2.1
12/8/2025	CM2	H2S	5.10%	1.40%	0.1
12/8/2025	CM2	NO	4.30%	3.80%	0.8
12/8/2025	CM2	NO2	1.50%	4.30%	1.4
12/8/2025	CM2	SO2	6.10%	2.70%	0.7
12/8/2025	CM2	Benzene	N/A	9.00%	0.4
12/8/2025	CM2	Toluene	N/A	2.30%	0.2
12/8/2025	CM2	Ethylbenzene	N/A	17.30%	0.7
12/8/2025	CM2	Xylenes	N/A	17.70%	1.5
12/15/2025	CM2	H2S	4.50%	0.50%	0.1
12/15/2025	CM2	NO	1.20%	2.70%	1.6
12/15/2025	CM2	NO2	3.70%	3.20%	1.8
12/15/2025	CM2	SO2	2.90%	1.10%	1.2
12/15/2025	CM2	Benzene	N/A	0.50%	0.4
12/15/2025	CM2	Toluene	N/A	0.30%	0.2
12/15/2025	CM2	Ethylbenzene	N/A	20.30%	0.5
12/15/2025	CM2	Xylenes	N/A	18.60%	2.2
12/22/2025	CM2	H2S	0.10%	27.10%	1.2
12/22/2025	CM2	NO	0.10%	30.80%	0
12/22/2025	CM2	NO2	6.10%	24.10%	2.3
12/22/2025	CM2	SO2	0.70%	27.50%	0.1
12/22/2025	CM2	Benzene	N/A	20.00%	0.3
12/22/2025	CM2	Toluene	N/A	20.50%	0.1
12/22/2025	CM2	Ethylbenzene	N/A	32.30%	0.5
12/22/2025	CM2	Xylenes	N/A	33.40%	1.5
12/29/2025	CM2	H2S	40.10%	1.20%	1.9
12/29/2025	CM2	NO	45.60%	5.90%	0.9
12/29/2025	CM2	NO2	17.70%	5.70%	1.2
12/29/2025	CM2	SO2	39.90%	5.20%	2.9
12/29/2025	CM2	Benzene	N/A	19.30%	0.7
12/29/2025	CM2	Toluene	N/A	19.80%	0.3
12/29/2025	CM2	Ethylbenzene	N/A	5.50%	1.2
12/29/2025	CM2	Xylenes	N/A	6.30%	2.4

Focus DETECT

Date	Location	Parameter	Precision (error)	Span (error)	Zero (absolute value)
10/6/2025	CM6	H2S	6.00%	9.80%	0.4
10/6/2025	CM6	NO	1.20%	1.20%	0.1
10/6/2025	CM6	NO2	4.30%	1.30%	2.3

10/6/2025	CM6	SO2	9.20%	10.60%	1
10/6/2025	CM6	Benzene	N/A	6.00%	0
10/6/2025	CM6	Toluene	N/A	4.00%	0
10/6/2025	CM6	Ethylbenzene	N/A	6.50%	0.3
10/6/2025	CM6	Xylenes	N/A	4.60%	2.6
10/13/2025	CM6	H2S	19.20%	3.60%	17
10/13/2025	CM6	NO	2.90%	0.60%	1.3
10/13/2025	CM6	NO2	6.00%	1.30%	1.8
10/13/2025	CM6	SO2	36.40%	14.30%	18.5
10/13/2025	CM6	Benzene	N/A	6.30%	0.2
10/13/2025	CM6	Toluene	N/A	1.80%	0.2
10/13/2025	CM6	Ethylbenzene	N/A	0.00%	0.4
10/13/2025	CM6	Xylenes	N/A	5.10%	1.8
10/20/2025	CM6	H2S	4.70%	0.70%	6.7
10/20/2025	CM6	NO	12.00%	9.70%	1.2
10/20/2025	CM6	NO2	5.20%	0.90%	1
10/20/2025	CM6	SO2	18.90%	16.10%	7.7
10/20/2025	CM6	Benzene	N/A	2.30%	0.1
10/20/2025	CM6	Toluene	N/A	13.00%	0.1
10/20/2025	CM6	Ethylbenzene	N/A	17.00%	0.8
10/20/2025	CM6	Xylenes	N/A	17.80%	1.3
10/27/2025	CM6	H2S	4.30%	7.70%	1.4
10/27/2025	CM6	NO	6.50%	11.10%	2.2
10/27/2025	CM6	NO2	2.10%	2.00%	0.2
10/27/2025	CM6	SO2	3.20%	10.30%	1.1
10/27/2025	CM6	Benzene	N/A	21.30%	0.3
10/27/2025	CM6	Toluene	N/A	8.00%	0
10/27/2025	CM6	Ethylbenzene	N/A	4.30%	0.6
10/27/2025	CM6	Xylenes	N/A	2.50%	3.2
11/3/2025	CM6	H2S	64.90%	17.10%	47.7
11/3/2025	CM6	NO	0.50%	1.00%	1.1
11/3/2025	CM6	NO2	3.90%	2.10%	1.5
11/3/2025	CM6	SO2	1.90%	1.00%	40.2
11/3/2025	CM6	Benzene	N/A	18.30%	0.1
11/3/2025	CM6	Toluene	N/A	0.30%	0.1
11/3/2025	CM6	Ethylbenzene	N/A	14.00%	0.9
11/3/2025	CM6	Xylenes	N/A	24.20%	3.3
11/10/2025	CM6	H2S	23.60%	33.10%	11.6
11/10/2025	CM6	NO	3.20%	0.80%	0.2
11/10/2025	CM6	NO2	0.40%	3.00%	1
11/10/2025	CM6	SO2	13.70%	26.60%	11.8
11/10/2025	CM6	Benzene	N/A	24.50%	0.1
11/10/2025	CM6	Toluene	N/A	9.00%	0.4
11/10/2025	CM6	Ethylbenzene	N/A	2.30%	0.3
11/10/2025	CM6	Xylenes	N/A	8.20%	1.8
11/17/2025	CM6	H2S	6.80%	4.20%	5.9

11/17/2025	CM6	NO	2.00%	4.40%	1.1
11/17/2025	CM6	NO2	3.10%	0.50%	1.9
11/17/2025	CM6	SO2	19.50%	11.70%	5.1
11/17/2025	CM6	Benzene	N/A	28.80%	0.3
11/17/2025	CM6	Toluene	N/A	11.80%	0.1
11/17/2025	CM6	Ethylbenzene	N/A	3.80%	1
11/17/2025	CM6	Xylenes	N/A	8.30%	1.5
11/24/2025	CM6	H2S	23.30%	7.30%	18.9
11/24/2025	CM6	NO	1.60%	0.80%	3.4
11/24/2025	CM6	NO2	4.00%	0.00%	0.7
11/24/2025	CM6	SO2	27.50%	10.90%	15.8
11/24/2025	CM6	Benzene	N/A	33.80%	0.1
11/24/2025	CM6	Toluene	N/A	14.80%	0.4
11/24/2025	CM6	Ethylbenzene	N/A	5.70%	0.9
11/24/2025	CM6	Xylenes	N/A	2.80%	2
12/1/2025	CM6	H2S	8.50%	6.50%	5.6
12/1/2025	CM6	NO	5.10%	1.50%	2.7
12/1/2025	CM6	NO2	3.90%	0.60%	1.1
12/1/2025	CM6	SO2	19.60%	14.30%	6.8
12/1/2025	CM6	Benzene	N/A	0.50%	0.2
12/1/2025	CM6	Toluene	N/A	8.80%	0.2
12/1/2025	CM6	Ethylbenzene	N/A	22.00%	0.9
12/1/2025	CM6	Xylenes	N/A	28.50%	1.9
12/8/2025	CM6	H2S	15.70%	7.60%	11.6
12/8/2025	CM6	NO	1.30%	9.00%	0
12/8/2025	CM6	NO2	3.60%	0.30%	0
12/8/2025	CM6	SO2	14.40%	7.80%	6.4
12/8/2025	CM6	Benzene	N/A	3.00%	0.1
12/8/2025	CM6	Toluene	N/A	1.30%	0.1
12/8/2025	CM6	Ethylbenzene	N/A	11.30%	0.5
12/8/2025	CM6	Xylenes	N/A	14.80%	1.8
12/15/2025	CM6	H2S	77.70%	84.70%	6.9
12/15/2025	CM6	NO	0.90%	0.10%	2.6
12/15/2025	CM6	NO2	1.50%	0.00%	0.2
12/15/2025	CM6	SO2	18.00%	12.20%	9.5
12/15/2025	CM6	Benzene	N/A	3.00%	0.2
12/15/2025	CM6	Toluene	N/A	6.80%	0.1
12/15/2025	CM6	Ethylbenzene	N/A	26.00%	0.8
12/15/2025	CM6	Xylenes	N/A	33.70%	1.4
12/22/2025	CM6	H2S	93.70%	98.70%	4.9
12/22/2025	CM6	NO	15.90%	28.50%	1.4
12/22/2025	CM6	NO2	5.10%	25.80%	0.1
12/22/2025	CM6	SO2	18.50%	13.20%	4.4
12/22/2025	CM6	Benzene	N/A	22.00%	0.1
12/22/2025	CM6	Toluene	N/A	22.30%	0.3
12/22/2025	CM6	Ethylbenzene	N/A	10.80%	0.5

12/22/2025	CM6	Xylenes	N/A	9.90%	1.7
12/29/2025	CM6	H2S	N/A	N/A	0
12/29/2025	CM6	NO	23.10%	4.40%	2.4
12/29/2025	CM6	NO2	7.10%	10.10%	2.1
12/29/2025	CM6	SO2	N/A	N/A	0
12/29/2025	CM6	Benzene	N/A	18.30%	0.1
12/29/2025	CM6	Toluene	N/A	11.00%	0.3
12/29/2025	CM6	Ethylbenzene	N/A	6.30%	0.4
12/29/2025	CM6	Xylenes	N/A	12.50%	1.8

Kearney DETECT

Date	Location	Parameter	Precision (error)	Span (error)	Zero (absolute value)
10/6/2025	CM7	H2S	3.20%	1.50%	0.4
10/6/2025	CM7	NO	6.80%	6.70%	0.2
10/6/2025	CM7	NO2	10.90%	3.80%	2.2
10/6/2025	CM7	SO2	4.10%	2.80%	0.4
10/6/2025	CM7	Benzene	N/A	1.80%	0.2
10/6/2025	CM7	Toluene	N/A	0.00%	0.1
10/6/2025	CM7	Ethylbenzene	N/A	16.30%	3.6
10/6/2025	CM7	Xylenes	N/A	30.20%	5.2
10/13/2025	CM7	H2S	3.70%	0.90%	0.3
10/13/2025	CM7	NO	4.90%	6.30%	0.3
10/13/2025	CM7	NO2	2.70%	15.10%	3.2
10/13/2025	CM7	SO2	3.90%	4.90%	0.4
10/13/2025	CM7	Benzene	N/A	19.80%	0.2
10/13/2025	CM7	Toluene	N/A	24.30%	0.3
10/13/2025	CM7	Ethylbenzene	N/A	1.50%	3.3
10/13/2025	CM7	Xylenes	N/A	3.60%	5.8
10/20/2025	CM7	H2S	3.10%	1.30%	0.5
10/20/2025	CM7	NO	5.50%	2.50%	0.6
10/20/2025	CM7	NO2	9.10%	0.70%	0
10/20/2025	CM7	SO2	4.30%	2.30%	0.3
10/20/2025	CM7	Benzene	N/A	5.00%	0
10/20/2025	CM7	Toluene	N/A	3.00%	0.3
10/20/2025	CM7	Ethylbenzene	N/A	23.30%	3
10/20/2025	CM7	Xylenes	N/A	21.00%	3.6
10/27/2025	CM7	H2S	4.10%	1.10%	0.3
10/27/2025	CM7	NO	4.70%	6.50%	0.2
10/27/2025	CM7	NO2	8.50%	0.30%	0.5
10/27/2025	CM7	SO2	3.50%	2.20%	0.4
10/27/2025	CM7	Benzene	N/A	31.50%	0.3
10/27/2025	CM7	Toluene	N/A	33.80%	0.2

10/27/2025	CM7	Ethylbenzene	N/A	44.00%	3
10/27/2025	CM7	Xylenes	N/A	45.70%	3.8
11/3/2025	CM7	H2S	4.00%	4.70%	0.4
11/3/2025	CM7	NO	3.20%	7.10%	1
11/3/2025	CM7	NO2	7.60%	2.70%	1.9
11/3/2025	CM7	SO2	2.70%	1.20%	0.4
11/3/2025	CM7	Benzene	N/A	23.50%	0.8
11/3/2025	CM7	Toluene	N/A	24.30%	0.8
11/3/2025	CM7	Ethylbenzene	N/A	6.80%	6.1
11/3/2025	CM7	Xylenes	N/A	1.80%	10.5
11/10/2025	CM7	H2S	4.10%	6.10%	0.3
11/10/2025	CM7	NO	4.80%	7.10%	0.5
11/10/2025	CM7	NO2	7.50%	3.40%	1.6
11/10/2025	CM7	SO2	3.90%	4.60%	0.4
11/10/2025	CM7	Benzene	N/A	32.50%	0.9
11/10/2025	CM7	Toluene	N/A	35.80%	0.6
11/10/2025	CM7	Ethylbenzene	N/A	13.30%	1.1
11/10/2025	CM7	Xylenes	N/A	7.30%	10.6
11/17/2025	CM7	H2S	5.20%	7.30%	0
11/17/2025	CM7	NO	2.10%	4.60%	1.8
11/17/2025	CM7	NO2	7.60%	8.70%	1
11/17/2025	CM7	SO2	3.60%	3.30%	0.6
11/17/2025	CM7	Benzene	N/A	19.00%	0.3
11/17/2025	CM7	Toluene	N/A	23.50%	0.1
11/17/2025	CM7	Ethylbenzene	N/A	9.30%	4.6
11/17/2025	CM7	Xylenes	N/A	8.00%	11.3
11/24/2025	CM7	H2S	4.00%	6.60%	0.1
11/24/2025	CM7	NO	4.10%	7.00%	0.4
11/24/2025	CM7	NO2	7.70%	2.20%	1.1
11/24/2025	CM7	SO2	2.50%	1.80%	0.5
11/24/2025	CM7	Benzene	N/A	20.80%	0.7
11/24/2025	CM7	Toluene	N/A	30.80%	0
11/24/2025	CM7	Ethylbenzene	N/A	2.30%	3.4
11/24/2025	CM7	Xylenes	N/A	1.20%	6.7
12/1/2025	CM7	H2S	3.70%	3.30%	0
12/1/2025	CM7	NO	4.30%	7.10%	1
12/1/2025	CM7	NO2	4.30%	3.90%	0
12/1/2025	CM7	SO2	3.10%	1.90%	0.6
12/1/2025	CM7	Benzene	N/A	16.50%	0.4
12/1/2025	CM7	Toluene	N/A	9.30%	0.1
12/1/2025	CM7	Ethylbenzene	N/A	1.50%	2.6
12/1/2025	CM7	Xylenes	N/A	4.30%	5.9
12/8/2025	CM7	H2S	3.70%	6.30%	0.1
12/8/2025	CM7	NO	3.30%	3.40%	0.3
12/8/2025	CM7	NO2	7.50%	1.80%	1
12/8/2025	CM7	SO2	3.90%	3.00%	0.6

12/8/2025	CM7	Benzene	N/A	4.00%	0.6
12/8/2025	CM7	Toluene	N/A	23.30%	0.2
12/8/2025	CM7	Ethylbenzene	N/A	23.50%	2.9
12/8/2025	CM7	Xylenes	N/A	27.30%	6.8
12/15/2025	CM7	H2S	4.80%	5.50%	0.1
12/15/2025	CM7	NO	2.30%	7.00%	0.2
12/15/2025	CM7	NO2	4.50%	1.80%	0.7
12/15/2025	CM7	SO2	3.60%	2.40%	0.6
12/15/2025	CM7	Benzene	N/A	9.80%	0.3
12/15/2025	CM7	Toluene	N/A	26.50%	0.9
12/15/2025	CM7	Ethylbenzene	N/A	29.30%	1.1
12/15/2025	CM7	Xylenes	N/A	31.40%	6.3
12/22/2025	CM7	H2S	11.20%	23.50%	0.2
12/22/2025	CM7	NO	14.30%	28.30%	1.2
12/22/2025	CM7	NO2	10.80%	27.90%	3.5
12/22/2025	CM7	SO2	15.60%	24.10%	0.3
12/22/2025	CM7	Benzene	N/A	22.50%	0.6
12/22/2025	CM7	Toluene	N/A	35.50%	0.4
12/22/2025	CM7	Ethylbenzene	N/A	35.30%	0.2
12/22/2025	CM7	Xylenes	N/A	26.10%	6.3
12/29/2025	CM7	H2S	14.30%	2.90%	0.3
12/29/2025	CM7	NO	12.50%	6.70%	0.8
12/29/2025	CM7	NO2	5.70%	27.40%	1.2
12/29/2025	CM7	SO2	13.90%	6.60%	0.6
12/29/2025	CM7	Benzene	N/A	25.80%	0.2
12/29/2025	CM7	Toluene	N/A	12.00%	1
12/29/2025	CM7	Ethylbenzene	N/A	27.30%	2.1
12/29/2025	CM7	Xylenes	N/A	45.50%	8.4

Monroe DETECT

Date	Location	Parameter	Precision (error)	Span (error)	Zero (absolute value)
10/6/2025	CM8	H2S	0.30%	0.20%	1.1
10/6/2025	CM8	NO	7.30%	6.30%	0.3
10/6/2025	CM8	NO2	15.90%	13.10%	1.6
10/6/2025	CM8	SO2	2.30%	3.30%	0.6
10/6/2025	CM8	Benzene	N/A	2.60%	0.2
10/6/2025	CM8	Toluene	N/A	0.40%	0.6
10/6/2025	CM8	Ethylbenzene	N/A	4.30%	0.4
10/6/2025	CM8	Xylenes	N/A	3.60%	1.9
10/13/2025	CM8	H2S	0.10%	0.30%	1
10/13/2025	CM8	NO	9.90%	5.20%	0.4
10/13/2025	CM8	NO2	2.00%	0.40%	1

10/13/2025	CM8	SO2	1.70%	1.40%	1.7
10/13/2025	CM8	Benzene	N/A	10.90%	0.3
10/13/2025	CM8	Toluene	N/A	6.80%	0.5
10/13/2025	CM8	Ethylbenzene	N/A	1.10%	0.7
10/13/2025	CM8	Xylenes	N/A	1.70%	0.8
10/20/2025	CM8	H2S	0.50%	0.00%	0.7
10/20/2025	CM8	NO	22.90%	9.80%	1.4
10/20/2025	CM8	NO2	0.50%	1.70%	2.4
10/20/2025	CM8	SO2	0.70%	1.10%	2
10/20/2025	CM8	Benzene	N/A	1.50%	0
10/20/2025	CM8	Toluene	N/A	13.30%	0.3
10/20/2025	CM8	Ethylbenzene	N/A	19.80%	0.5
10/20/2025	CM8	Xylenes	N/A	25.70%	1.4
10/27/2025	CM8	H2S	N/A	N/A	1.1
10/27/2025	CM8	NO	18.00%	15.90%	0
10/27/2025	CM8	NO2	1.30%	0.20%	1
10/27/2025	CM8	SO2	1.90%	2.60%	1.3
10/27/2025	CM8	Benzene	N/A	11.30%	0.2
10/27/2025	CM8	Toluene	N/A	5.00%	0.3
10/27/2025	CM8	Ethylbenzene	N/A	3.00%	0.2
10/27/2025	CM8	Xylenes	N/A	5.20%	3.4
11/3/2025	CM8	H2S	12.90%	46.40%	0.6
11/3/2025	CM8	NO	7.50%	5.50%	0.1
11/3/2025	CM8	NO2	0.40%	2.10%	0
11/3/2025	CM8	SO2	2.10%	4.00%	1.3
11/3/2025	CM8	Benzene	N/A	34.00%	0.2
11/3/2025	CM8	Toluene	N/A	28.50%	0.3
11/3/2025	CM8	Ethylbenzene	N/A	23.80%	0.2
11/3/2025	CM8	Xylenes	N/A	19.80%	3.4
11/10/2025	CM8	H2S	21.50%	11.40%	0.8
11/10/2025	CM8	NO	4.80%	2.80%	2
11/10/2025	CM8	NO2	4.80%	6.50%	5.6
11/10/2025	CM8	SO2	1.50%	2.20%	1.1
11/10/2025	CM8	Benzene	N/A	N/A	0.3
11/10/2025	CM8	Toluene	N/A	N/A	0.2
11/10/2025	CM8	Ethylbenzene	N/A	N/A	1
11/10/2025	CM8	Xylenes	N/A	N/A	2.1
11/17/2025	CM8	H2S	6.50%	4.80%	0.2
11/17/2025	CM8	NO	13.70%	16.30%	0.5
11/17/2025	CM8	NO2	7.60%	1.50%	6
11/17/2025	CM8	SO2	1.70%	3.30%	0.7
11/17/2025	CM8	Benzene	N/A	N/A	0.2
11/17/2025	CM8	Toluene	N/A	N/A	0.3
11/17/2025	CM8	Ethylbenzene	N/A	N/A	0.4
11/17/2025	CM8	Xylenes	N/A	N/A	2.1
11/24/2025	CM8	H2S	6.00%	5.00%	0.8

11/24/2025	CM8	NO	15.10%	15.40%	1.1
11/24/2025	CM8	NO2	2.80%	0.80%	1.2
11/24/2025	CM8	SO2	3.50%	3.50%	1.2
11/24/2025	CM8	Benzene	N/A	N/A	0.1
11/24/2025	CM8	Toluene	N/A	N/A	0.2
11/24/2025	CM8	Ethylbenzene	N/A	N/A	0.3
11/24/2025	CM8	Xylenes	N/A	N/A	2
12/1/2025	CM8	H2S	6.80%	6.00%	0.5
12/1/2025	CM8	NO	10.90%	8.80%	0.1
12/1/2025	CM8	NO2	0.40%	2.30%	1
12/1/2025	CM8	SO2	3.50%	0.70%	1.4
12/1/2025	CM8	Benzene	N/A	11.00%	0.3
12/1/2025	CM8	Toluene	N/A	11.80%	0.4
12/1/2025	CM8	Ethylbenzene	N/A	19.80%	0.2
12/1/2025	CM8	Xylenes	N/A	15.30%	2.8
12/8/2025	CM8	H2S	6.30%	5.00%	0.3
12/8/2025	CM8	NO	8.10%	10.00%	1.3
12/8/2025	CM8	NO2	2.40%	0.30%	1
12/8/2025	CM8	SO2	2.30%	1.30%	0.9
12/8/2025	CM8	Benzene	N/A	N/A	0.1
12/8/2025	CM8	Toluene	N/A	N/A	0.1
12/8/2025	CM8	Ethylbenzene	N/A	N/A	1
12/8/2025	CM8	Xylenes	N/A	N/A	0.9
12/15/2025	CM8	H2S	5.50%	4.30%	0.2
12/15/2025	CM8	NO	2.70%	0.70%	1.4
12/15/2025	CM8	NO2	0.80%	1.00%	2
12/15/2025	CM8	SO2	1.90%	1.90%	1
12/15/2025	CM8	Benzene	N/A	47.50%	0.3
12/15/2025	CM8	Toluene	N/A	66.00%	0.5
12/15/2025	CM8	Ethylbenzene	N/A	62.80%	1
12/15/2025	CM8	Xylenes	N/A	72.80%	1
12/22/2025	CM8	H2S	10.70%	25.10%	26.4
12/22/2025	CM8	NO	8.50%	20.00%	0.8
12/22/2025	CM8	NO2	4.70%	18.70%	8.1
12/22/2025	CM8	SO2	3.70%	17.50%	0.9
12/22/2025	CM8	Benzene	N/A	N/A	0.7
12/22/2025	CM8	Toluene	N/A	N/A	0.6
12/22/2025	CM8	Ethylbenzene	N/A	N/A	1.8
12/22/2025	CM8	Xylenes	N/A	N/A	0.5
12/29/2025	CM8	H2S	N/A	N/A	N/A
12/29/2025	CM8	NO	N/A	N/A	N/A
12/29/2025	CM8	NO2	N/A	N/A	N/A
12/29/2025	CM8	SO2	N/A	N/A	N/A
12/29/2025	CM8	Benzene	N/A	N/A	N/A
12/29/2025	CM8	Toluene	N/A	N/A	N/A
12/29/2025	CM8	Ethylbenzene	N/A	N/A	N/A

12/29/2025	CM8	Xylenes	N/A	N/A	N/A
------------	-----	---------	-----	-----	-----

Alsup DETECT

Date	Location	Parameter	Precision (error)	Span (error)	Zero (absolute value)
10/6/2025	CM10	H2S	2.90%	3.60%	0.1
10/6/2025	CM10	NO	4.00%	0.50%	0.1
10/6/2025	CM10	NO2	6.70%	17.70%	3.6
10/6/2025	CM10	SO2	1.10%	6.20%	1.1
10/6/2025	CM10	Benzene	N/A	12.80%	1.1
10/6/2025	CM10	Toluene	N/A	9.00%	0.2
10/6/2025	CM10	Ethylbenzene	N/A	4.30%	2.3
10/6/2025	CM10	Xylenes	N/A	8.10%	5
10/13/2025	CM10	H2S	3.50%	2.10%	0.6
10/13/2025	CM10	NO	3.50%	3.70%	1
10/13/2025	CM10	NO2	12.00%	1.40%	3.2
10/13/2025	CM10	SO2	2.50%	6.00%	0.4
10/13/2025	CM10	Benzene	N/A	N/A	N/A
10/13/2025	CM10	Toluene	N/A	N/A	N/A
10/13/2025	CM10	Ethylbenzene	N/A	N/A	N/A
10/13/2025	CM10	Xylenes	N/A	N/A	N/A
10/20/2025	CM10	H2S	1.30%	5.10%	0.3
10/20/2025	CM10	NO	0.40%	0.30%	0.7
10/20/2025	CM10	NO2	84.70%	0.20%	3.6
10/20/2025	CM10	SO2	2.90%	4.70%	0.1
10/20/2025	CM10	Benzene	N/A	N/A	N/A
10/20/2025	CM10	Toluene	N/A	N/A	N/A
10/20/2025	CM10	Ethylbenzene	N/A	N/A	N/A
10/20/2025	CM10	Xylenes	N/A	N/A	N/A
10/27/2025	CM10	H2S	0.30%	7.60%	0.6
10/27/2025	CM10	NO	2.40%	0.30%	0.7
10/27/2025	CM10	NO2	1.10%	6.80%	0.1
10/27/2025	CM10	SO2	2.70%	0.50%	0.4
10/27/2025	CM10	Benzene	N/A	N/A	2
10/27/2025	CM10	Toluene	N/A	N/A	0.7
10/27/2025	CM10	Ethylbenzene	N/A	N/A	2.3
10/27/2025	CM10	Xylenes	N/A	N/A	8
11/3/2025	CM10	H2S	1.30%	5.90%	0.6
11/3/2025	CM10	NO	3.10%	0.20%	1
11/3/2025	CM10	NO2	3.50%	2.00%	1.6
11/3/2025	CM10	SO2	4.00%	4.70%	0.3
11/3/2025	CM10	Benzene	N/A	N/A	3.4
11/3/2025	CM10	Toluene	N/A	N/A	2.5

11/3/2025	CM10	Ethylbenzene	N/A	N/A	1.9
11/3/2025	CM10	Xylenes	N/A	N/A	4.1
11/10/2025	CM10	H2S	2.80%	2.40%	0.4
11/10/2025	CM10	NO	4.80%	1.30%	0.2
11/10/2025	CM10	NO2	1.90%	1.20%	2.9
11/10/2025	CM10	SO2	1.90%	4.60%	0.2
11/10/2025	CM10	Benzene	N/A	N/A	3.2
11/10/2025	CM10	Toluene	N/A	N/A	1
11/10/2025	CM10	Ethylbenzene	N/A	N/A	3
11/10/2025	CM10	Xylenes	N/A	N/A	5.9
11/17/2025	CM10	H2S	1.60%	5.30%	0.5
11/17/2025	CM10	NO	4.00%	2.80%	2.3
11/17/2025	CM10	NO2	6.50%	8.20%	4.2
11/17/2025	CM10	SO2	1.30%	5.30%	0.3
11/17/2025	CM10	Benzene	N/A	N/A	0
11/17/2025	CM10	Toluene	N/A	N/A	0
11/17/2025	CM10	Ethylbenzene	N/A	N/A	0
11/17/2025	CM10	Xylenes	N/A	N/A	0
11/24/2025	CM10	H2S	2.10%	6.20%	0.5
11/24/2025	CM10	NO	8.90%	11.00%	2.8
11/24/2025	CM10	NO2	10.10%	0.10%	2.8
11/24/2025	CM10	SO2	4.50%	5.10%	0.2
11/24/2025	CM10	Benzene	N/A	N/A	3.1
11/24/2025	CM10	Toluene	N/A	N/A	0.6
11/24/2025	CM10	Ethylbenzene	N/A	N/A	2.9
11/24/2025	CM10	Xylenes	N/A	N/A	5.6
12/1/2025	CM10	H2S	1.90%	2.30%	0.5
12/1/2025	CM10	NO	3.50%	0.20%	0.3
12/1/2025	CM10	NO2	4.90%	1.30%	2.5
12/1/2025	CM10	SO2	2.40%	5.30%	0.1
12/1/2025	CM10	Benzene	N/A	N/A	2.7
12/1/2025	CM10	Toluene	N/A	N/A	1.6
12/1/2025	CM10	Ethylbenzene	N/A	N/A	2.9
12/1/2025	CM10	Xylenes	N/A	N/A	3.9
12/8/2025	CM10	H2S	1.70%	4.10%	0.8
12/8/2025	CM10	NO	8.30%	4.70%	0.3
12/8/2025	CM10	NO2	8.00%	4.30%	2
12/8/2025	CM10	SO2	7.50%	4.60%	0.4
12/8/2025	CM10	Benzene	N/A	N/A	2.1
12/8/2025	CM10	Toluene	N/A	N/A	2.1
12/8/2025	CM10	Ethylbenzene	N/A	N/A	2
12/8/2025	CM10	Xylenes	N/A	N/A	3
12/15/2025	CM10	H2S	5.60%	3.40%	0.4
12/15/2025	CM10	NO	3.90%	0.20%	0.5
12/15/2025	CM10	NO2	10.10%	0.80%	2.6
12/15/2025	CM10	SO2	0.50%	3.50%	0.5

12/15/2025	CM10	Benzene	N/A	N/A	4.2
12/15/2025	CM10	Toluene	N/A	N/A	2.9
12/15/2025	CM10	Ethylbenzene	N/A	N/A	2.6
12/15/2025	CM10	Xylenes	N/A	N/A	3.5
12/22/2025	CM10	H2S	5.70%	14.00%	0.4
12/22/2025	CM10	NO	21.90%	24.20%	1.5
12/22/2025	CM10	NO2	26.50%	21.70%	1
12/22/2025	CM10	SO2	25.50%	22.50%	0.5
12/22/2025	CM10	Benzene	N/A	24.30%	0
12/22/2025	CM10	Toluene	N/A	22.50%	0
12/22/2025	CM10	Ethylbenzene	N/A	22.00%	0
12/22/2025	CM10	Xylenes	N/A	25.30%	0.3
12/29/2025	CM10	H2S	15.30%	0.50%	1.8
12/29/2025	CM10	NO	1.20%	6.80%	1.4
12/29/2025	CM10	NO2	9.60%	9.00%	1.7
12/29/2025	CM10	SO2	34.10%	7.80%	2.8
12/29/2025	CM10	Benzene	N/A	38.30%	0
12/29/2025	CM10	Toluene	N/A	31.50%	0
12/29/2025	CM10	Ethylbenzene	N/A	30.00%	0
12/29/2025	CM10	Xylenes	N/A	30.30%	0.2

Rose Hill

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM1	10/6/2025	5.20%	22.00%	2.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	56.00%
CM1	11/14/2025	14.20%	26.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	29.00%
CM1	12/3/2025	10.40%	16.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	14.00%

RBC

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM2	10/8/2025	11.50%	6.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	4.00%
CM2	11/4/2025	2.40%	190.00%	2.40%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	2.00%
CM2	12/1/2025	29.20%	60.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	2.00%

Adams
High

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM3	10/22/2025	20.80%	1.00%	1.00%	5.00%	4.00%	5.50%	14.75%	17.00%	0.00%	6.75%	1.00%	0.00%	26.00%
CM3	11/18/2025	29.20%	27.00%	0.30%	6.00%	2.00%	0.00%	16.00%	16.00%	0.00%	7.00%	1.00%	0.00%	21.00%
CM3	12/18/2025	33.60%	45.00%	0.00%	12.00%	9.00%	0.00%	4.25%	2.00%	0.00%	5.00%	5.00%	0.50%	19.00%

Adams
Middle

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM4	10/9/2025	29.60%	77.00%	0.00%	21.50%	25.00%	0.50%	26.00%	24.00%	2.50%	0.25%	16.00%	0.00%	20.00%
CM4	11/14/2025	35.00%	80.00%	0.00%	5.00%	0.00%	2.50%	15.50%	13.00%	2.50%	11.00%	4.00%	0.00%	13.00%
CM4	12/5/2025	5.00%	50.00%	0.00%	25.00%	28.00%	0.50%	7.75%	70.00%	2.50%	0.75%	16.00%	1.00%	16.00%

Central

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM5	10/20/2025	15.80%	12.00%	1.00%	4.00%	11.00%	2.50%	2.75%	46.00%	0.00%	2.25%	12.00%	1.00%	13.00%
CM5	11/17/2025	18.20%	2.00%	0.60%	1.50%	6.00%	0.00%	3.50%	18.00%	0.00%	4.00%	8.00%	0.75%	9.00%
CM5	12/4/2025	5.80%	100.00%	1.50%	15.00%	26.00%	0.50%	10.75%	53.00%	0.00%	6.75%	16.00%	0.00%	14.00%

Focus
Point

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM6	10/21/2025	23.20%	26.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	2.00%
CM6	11/19/2025	29.40%	34.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	2.00%
CM6	12/15/2025	7.00%	14.00%	1.40%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	3.00%

Kearney Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM7	10/21/2025	11.00%	2.00%	1.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	0.00%
CM7	11/19/2025	17.00%	21.00%	0.60%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	1.00%
CM7	12/15/2025	11.50%	1.00%	1.90%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	5.00%

Monroe Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM8	10/6/2025	8.50%	14.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	8.00%
CM8	11/3/2025	22.00%	28.00%	0.50%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	5.00%
CM8	12/3/2025	9.00%	2.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	4.00%

Riverside Cemetery Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM9	10/3/2025	21.80%	7.00%	0.00%	3.50%	10.00%	3.50%	53.75%	37.00%	2.50%	9.75%	28.00%	2.75%	13.00%
CM9	11/6/2025	16.40%	32.00%	0.00%	6.50%	3.00%	4.00%	30.25%	50.00%	0.00%	6.25%	15.00%	1.00%	8.00%
CM9	12/2/2025	2.80%	50.00%	1.00%	8.00%	8.00%	2.50%	16.50%	14.00%	2.50%	12.75%	19.00%	0.00%	18.00%

Alsup

Sensit RAMP

		Validation Results Table												
		CO Error			NO2 Error			SO2 Error			H2S Error			VOC Error
Community Monitor Location	Validation Date	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Span (<30%)	Precision (<30%)	Zero (<10%)	Precision (<30%)
CM10	10/22/2025	14.80%	43.00%	0.20%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	36.00%
CM10	11/20/2025	9.20%	13.00%	0.20%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	40.00%
CM10	12/18/2025	18.50%	69.00%	0.00%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A	79.00%

Appendix B Field Data Sheets

AQM Serial Number	829	830	831
Community Monitor Location	2	7	6
Date	12/23/2025	12/12/2025	12/12/2025
Operator	AT	AT	AT

Monthly Checks

CO bottle (psi)	✓	✓	✓
TVOC bottle (psi)	✓	✓	✓
Gas Validation Checks (weekly, reviewed Monthly)	✓	✓	✓

Quarterly Checks

Gas Inlet

Flow Rate	✓	✓	✓
Filter Change	✓	✓	✓
Field Calibration (H2S, SO2)	✓	✓	✓

Particulate Monitor

Flow Rate	✓	✓	✓
Filter Change	✓	✓	✓
Check for Leaks	✓	✓	✓
Check Zero (+/- 3.0 ug/m ³)	✓	✓	✓
Check laser and detector (17.6 mA)	✓	✓	✓
Clean Cyclone	✓	✓	✓

Appendix C Calibration Gas Certification Sheets



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 22065913
Lot Number: 304-402577436-1

Customer: Cal Gas Direct Inc.
Use Before: 10/28/2026

Component	Requested Concentration	Analytical Result (+/- 2%)
Isobutylene	200 PPM	206.1 PPM
Nitrogen	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:


Glenn Velez



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 22070686
Lot Number: 304-402651362-1

Customer: Cal Gas Direct Inc.
Use Before: 02/01/2025

Component	Requested Concentration	Analytical Result (+/- 2%)
Hydrogen Sulfide	20 PPM	20 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:


Glenn Velez



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: February 6, 2024
Order Number: 24090699
Lot Number: 304-402960511-1

Customer: Cal Gas Direct Inc.
Use Before: 02/06/2026

<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Sulfur Dioxide	20 PPM	21.6 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:


Kendall Gaspard



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: February 6, 2024
Order Number: 24090699
Lot Number: 304-402960512-1

Customer: Cal Gas Direct Inc.
Use Before: 02/06/2028


Component	Requested Concentration	Analytical Result (+/- 2%)
Carbon Monoxide	500 PPM	492 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:


Kendall Gaspard



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24093799
Lot Number: 304-403009405-1

Customer: Cal Gas Direct Inc.
Use Before: 04/02/2028

<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Isobutylene	200 PPM	207.4 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:

Matthew Creighton
MATTHEW CREIGHTON



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24102390
Lot Number: 304-403151303-1

Customer: Cal Gas Direct Inc.
Use Before: 09/20/2026

Component	Requested Concentration	Analytical Result (+/- 5%)
Sulfur Dioxide	20 PPM	18.5 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:


Glenn Velez



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24102390
Lot Number: 304-403151305-1

Customer: Cal Gas Direct Inc.
Use Before: 09/20/2026

Component	Requested Concentration	Analytical Result (+/- 5%)
Hydrogen Sulfide	20 PPM	21 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:


Glenn Velez



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24111624
Lot Number: 304-403296511-1

Customer: Cal Gas Direct Inc.
Use Before: 03/17/2027

<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 5%)</u>
Sulfur Dioxide	20 PPM	19.1 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24111624
Lot Number: 304-403296512-1

Customer: Cal Gas Direct Inc.
Use Before: 03/17/2027

Component	Requested Concentration	Analytical Result (+/- 5%)
Hydrogen Sulfide	20 PPM	21 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24111624
Lot Number: 304-403296513-1

Customer: Cal Gas Direct Inc.
Use Before: 03/17/2029

<u>Component</u>	<u>Requested Concentration</u>	<u>Analytical Result (+/- 2%)</u>
Carbon Monoxide	500 PPM	515 PPM
Nitrogen	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:



GASCO AFFILIATES, LLC.

320 Scarlet Blvd.
Oldsmar, FL 34677
(800) 910-0051
fax: (866) 755-8920
www.gascogas.com

CERTIFICATE OF ANALYSIS

Date: June 10, 2026
Order Number: 24111632
Lot Number: 304-403297204-1

Customer: Cal Gas Direct Inc.
Use Before: 03/16/2029

Component	Requested Concentration	Analytical Result (+/- 2%)
Isobutylene	200 PPM	206 PPM
Air	Balance	Balance

Cylinder Size: 2.0 Cu. Ft.
Contents: 58 Liter

Valve: 5/8" -18UNF
Pressure: 500 psig

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

Analyst:

Edraira Colon



GASCO AFFILIATES, LLC.
 320 Scarlet Blvd.
 Oldsmar, FL 34677
 (800) 910-0051
 www.gasco-gas.com

CERTIFICATE OF ANALYSIS

Date: 05/15/2025
Order Number: 24113589
Lot Number: 304-403347151-1

Customer: CAL GAS DIRECT INC
Part Number: X02NI99CP585871
Use Before: 05/15/2029

<u>Components</u>	<u>Concentration (mole %)</u>	<u>Relative Tolerance</u>
CARBON MONOXIDE (CO)	500 PPM	±2%
NITROGEN (N2)	BALANCE	

Pressure: 500 PSIG @ 70° F

Valve: 5/8"-18UNF (C10)

Cylinder Contents, Cylinder Size: 2.05 Cu. Ft., 58L

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:

Darar Reyes
Darar Reyes



GASCO AFFILIATES, LLC.
 320 Scarlet Blvd.
 Oldsmar, FL 34677
 (800) 910-0051
 www.gasco-gas.com

CERTIFICATE OF ANALYSIS

Date: 05/15/2025
Order Number: 24113589
Lot Number: 304-403347152-1

Customer: CAL GAS DIRECT INC
Part Number: X02AI99CP584438
Use Before: 05/15/2027

<u>Components</u>	<u>Concentration (mole %)</u>	<u>Relative Tolerance</u>
HYDROGEN SULFIDE (H2S)	20 PPM	±10%
AIR (20.9% Oxygen in Nitrogen)	BALANCE	

Pressure: 500 PSIG @ 70° F

Valve: 5/8"-18UNF (C10)

Cylinder Contents, Cylinder Size: 2.05 Cu. Ft., 58L

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:

Omar Reyes
Omar Reyes



GASCO AFFILIATES, LLC.
 320 Scarlet Blvd.
 Oldsmar, FL 34677
 (800) 910-0051
 www.gasco-gas.com

CERTIFICATE OF ANALYSIS

Date: 05/15/2025
Order Number: 24113589
Lot Number: 304-403347153-1

Customer: CAL GAS DIRECT INC
Part Number: X02AI99CP5851A5
Use Before: 05/15/2027

Components	Concentration (mole %)	Relative Tolerance
SULFUR DIOXIDE (SO ₂)	20 PPM	±10%
AIR (20.9% Oxygen in Nitrogen)	BALANCE	

Pressure: 500 PSIG @ 70° F

Valve: 5/8"-18UNF (C10)

Cylinder Contents, Cylinder Size: 2.05 Cu. Ft., 58L

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/ or N.I.S.T. Gas Mixture reference materials.

Analyst:

Omar Reyes
Omar Reyes

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E02NI99E15A3168	Reference Number: 153-402623607-1
Cylinder Number: CC69278	Cylinder Volume: 144.0 CF
Laboratory: 124 - Tooele (SAP) - UT	Cylinder Pressure: 2015 PSIG
PGVP Number: B72023	Valve Outlet: 350
Gas Code: CO,BALN	Certification Date: Jan 04, 2023

Expiration Date: Jan 04, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
CARBON MONOXIDE	500.0 PPM	502.7 PPM	G1	+/- 0.8% NIST Traceable	01/04/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	15060543	CC453965	491.9 PPM CARBON MONOXIDE/NITROGEN	0.6	Mar 05, 2027

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2110269 CO MCO	FTIR	Dec 22, 2022

Triad Data Available Upon Request



Signature on file
Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Part Number:	X02NI99C20000E4	Reference Number:	160-403345933-1
Cylinder Number:	A025022	Cylinder Volume:	215.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2014 PSIG
Analysis Date:	May 14, 2025	Valve Outlet:	350
Lot Number:	160-403345933-1		

Expiration Date: May 14, 2028

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
ISOBUTYLENE	200.0 PPM	203.4 PPM	+/-2%
NITROGEN	Balance		





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Part Number:	X02NI99C15A17E7	Reference Number:	153-403347775-1
Cylinder Number:	ALM036564	Cylinder Volume:	144.0 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	2015 PSIG
Analysis Date:	May 27, 2025	Valve Outlet:	660
Lot Number:	153-403347775-1		

Expiration Date: May 27, 2033

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
SULFUR DIOXIDE	20.00 PPM	20.38 PPM	+/- 5%
NITROGEN	Balance		





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer:	MONTROSE AIR QUALITY SERVICES LLC -	Reference Number:	126-403345430-1
Part Number:	X02NI99C15A0312	Cylinder Volume:	144.3 CF
Cylinder Number:	CC268099	Cylinder Pressure:	2015 PSIG
Laboratory:	124 - La Porte Mix - TX	Valve Outlet:	330
Analysis Date:	Jun 05, 2025		
Lot Number:	126-403345430-1		

Expiration Date: Jun 05, 2028

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
HYDROGEN SULFIDE	20.00 PPM	19.41 PPM	± 5%
NITROGEN	Balance		

Notes:
PO NUMBER: 078165



Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E03NI99E33A00K9	Reference Number: 153-403128093-1
Cylinder Number: FF41970	Cylinder Volume: 31.6 CF
Laboratory: 124 - Tooele (SAP) - UT	Cylinder Pressure: 2217 PSIG
PGVP Number: B72024	Valve Outlet: 660
Gas Code: NO,NOX,SO2,BALN	Certification Date: Sep 03, 2024

Expiration Date: Sep 03, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	40.00 PPM	39.62 PPM	G1	+/- 1.1% NIST Traceable	08/26/2024, 09/03/2024
SULFUR DIOXIDE	40.00 PPM	39.60 PPM	G1	+/- 0.8% NIST Traceable	08/26/2024, 09/03/2024
NITRIC OXIDE	40.00 PPM	39.58 PPM	G1	+/- 1.2% NIST Traceable	08/26/2024, 09/03/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	DCK01201202249	CC750448	49.13 PPM NITRIC OXIDE/NITROGEN	0.5%	May 03, 2026
PRM	12404	APEX1324257	50.04 PPM NITRIC OXIDE/NITROGEN	0.4%	Dec 22, 2023
GMIS	1531022022103	CC517868	4.914 PPM NITROGEN DIOXIDE/NITROGEN	1.6%	Feb 17, 2026
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	1.5%	Feb 17, 2023
GMIS	072120222A114	EB0141223	49.87 PPM SULFUR DIOXIDE/NITROGEN	0.7%	Dec 21, 2026
SRM	12431	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	0.6%	Jun 27, 2023

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010228 NO LNO	FTIR	Aug 28, 2024
Nicolet iS50 AUP2010228 NO2 impurity	FTIR NO2 impurity	Aug 28, 2024
Nicolet iS50 AUP2010228 SO2 LSO2	FTIR	Aug 22, 2024

Triad Data Available Upon Request



 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33W0030	Reference Number:	54-403219688-1
Cylinder Number:	D526138	Cylinder Volume:	32.0 CF
Laboratory:	124 - Chicago (SAP) - IL	Cylinder Pressure:	2215 PSIG
PGVP Number:	B12025	Valve Outlet:	660
Gas Code:	NO2,BALN	Certification Date:	Jan 06, 2025

Expiration Date: Jan 06, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NITROGEN DIOXIDE	40.00 PPM	41.24 PPM	G1	+/- 2.1% NIST Traceable	12/27/2024, 01/06/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	1534002024501	CC500127	59.33 PPM NITROGEN DIOXIDE/AIR	+/- 1.8%	Apr 04, 2027
PRM	12438	D153564	59.5 PPM NITROGEN DIOXIDE/AIR	+/- 1.7%	Nov 21, 2024

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR NO2 017707558	FTIR	Jan 03, 2025

Triad Data Available Upon Request

PERMANENT NOTES: OXYGEN ADDED TO MAINTAIN STABILITY.




 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - HENDERSON ,
CO

Part X07NI99C33A0033

Number:

Cylinder FF37325

Number:

Laboratory: 124 - La Porte Mix - TX

Analysis Oct 09, 2024

Date:

Lot Number: 126-403147050-1

Reference Number: 126-403147050-1

Cylinder Volume: 308.0 CF

Cylinder Pressure: 2216 PSIG

Valve Outlet: 350

Expiration Date: Oct 09, 2027

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	20.00 PPM	19.00 PPM	+/-5%
ETHYL BENZENE	20.00 PPM	19.69 PPM	+/-5%
TOLUENE	20.00 PPM	19.50 PPM	+/-5%
M XYLENE	20.00 PPM	19.89 PPM	+/-5%
O XYLENE	20.00 PPM	19.86 PPM	+/-5%
P XYLENE	20.00 PPM	19.89 PPM	+/-5%
NITROGEN	Balance		

Notes: MONTROSE AIR QUALITY SERVICES LLC

PO#: 62293





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - C264

HENDERSON, CO

Part X06NI99C33A0054

Reference Number: 126-403465624-1

Number:

Cylinder FF39327

Cylinder Volume: 31.6 CF

Number:

Laboratory: 124 - La Porte Mix - TX

Cylinder Pressure: 2217 PSIG

Analysis Nov 14, 2025

Valve Outlet: 350

Date:

Lot Number: 126-403465624-1

Expiration Date: Nov 14, 2028

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	2.000 PPM	2.005 PPM	± 5%
ETHYL BENZENE	2.000 PPM	1.889 PPM	± 5%
M XYLENE	1.000 PPM	0.9175 PPM	± 5%
P XYLENE	1.000 PPM	0.9200 PPM	± 5%
TOLUENE	2.000 PPM	1.960 PPM	± 5%
NITROGEN	Balance		

Notes:

PO NUMBER: 078165





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E02NI99E33A00Q0	Reference Number: 160-403128091-1
Cylinder Number: FF44588	Cylinder Volume: 31.6 CF
Laboratory: 124 - Plumsteadville - PA	Cylinder Pressure: 2217 PSIG
PGVP Number: A12024	Valve Outlet: 330
Gas Code: H2S,BALN	Certification Date: Sep 04, 2024

Expiration Date: Sep 04, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	40.48 PPM	G1	+/- 2.0% NIST Traceable	08/27/2024, 09/04/2024
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	122401193440108	CC440120	49.49 PPM HYDROGEN SULFIDE/NITROGEN	+/-1.6%	Sep 28, 2026
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Aug 15, 2024

Triad Data Available Upon Request




 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02N199E33W0030	Reference Number:	54-403219688-1
Cylinder Number:	D049939	Cylinder Volume:	32.0 CF
Laboratory:	124 - Chicago (SAP) - IL	Cylinder Pressure:	2215 PSIG
PGVP Number:	B12025	Valve Outlet:	660
Gas Code:	NO2,BALN	Certification Date:	Jan 06, 2025

Expiration Date: Jan 06, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NITROGEN DIOXIDE	40.00 PPM	41.43 PPM	G1	+/- 2.1% NIST Traceable	12/27/2024, 01/06/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	1534002024501	CC500127	59.33 PPM NITROGEN DIOXIDE/AIR	+/- 1.8%	Apr 04, 2027
PRM	12438	D153564	59.5 PPM NITROGEN DIOXIDE/AIR	+/- 1.7%	Nov 21, 2024

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR NO2 017707558	FTIR	Jan 03, 2025

Triad Data Available Upon Request

PERMANENT NOTES: OXYGEN ADDED TO MAINTAIN STABILITY.





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - C264

HENDERSON, CO

Part X07NI99C33A0037

Reference Number: 126-403339419-1

Number:

Cylinder EX0015548

Cylinder Volume: 31.6 CF

Number:

Laboratory: 124 - La Porte Mix - TX

Cylinder Pressure: 2217 PSIG

Analysis Jun 12, 2025

Valve Outlet: 350SS

Date:

Lot Number: 126-403339419-1

Expiration Date: Jun 12, 2028

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	2.000 PPM	2.005 PPM	± 5%
ETHYL BENZENE	2.000 PPM	1.956 PPM	± 5%
M XYLENE	2.000 PPM	1.910 PPM	± 5%
O XYLENE	2.000 PPM	1.915 PPM	± 5%
P XYLENE	2.000 PPM	1.952 PPM	± 5%
TOLUENE	2.000 PPM	1.968 PPM	± 5%
NITROGEN	Balance		

Notes:.

PO NUMBER: 078165



Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E03NI99E33A00K9	Reference Number:	153-403128093-1
Cylinder Number:	FF49738	Cylinder Volume:	31.6 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	2217 PSIG
PGVP Number:	B72024	Valve Outlet:	660
Gas Code:	NO,NOX,SO2,BALN	Certification Date:	Sep 03, 2024

Expiration Date: Sep 03, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	40.00 PPM	39.59 PPM	G1	+/- 1.1% NIST Traceable	08/26/2024, 09/03/2024
SULFUR DIOXIDE	40.00 PPM	39.62 PPM	G1	+/- 0.8% NIST Traceable	08/26/2024, 09/03/2024
NITRIC OXIDE	40.00 PPM	39.59 PPM	G1	+/- 1.1% NIST Traceable	08/26/2024, 09/03/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	DCK01201202249	CC750448	49.13 PPM NITRIC OXIDE/NITROGEN	0.5%	May 03, 2026
PRM	12404	APEX1324257	50.04 PPM NITRIC OXIDE/NITROGEN	0.4%	Dec 22, 2023
GMIS	1531022022103	CC517868	4.914 PPM NITROGEN DIOXIDE/NITROGEN	1.6%	Feb 17, 2026
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	1.5%	Feb 17, 2023
GMIS	072120222A114	EB0141223	49.87 PPM SULFUR DIOXIDE/NITROGEN	0.7%	Dec 21, 2026
SRM	12431	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	0.6%	Jun 27, 2023

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010228 NO LNO	FTIR	Aug 28, 2024
Nicolet iS50 AUP2010228 NO2 impurity	FTIR NO2 impurity	Aug 28, 2024
Nicolet iS50 AUP2010228 SO2 LSO2	FTIR	Aug 22, 2024

Triad Data Available Upon Request





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E02NI99E33A00Q0	Reference Number: 160-403128091-1
Cylinder Number: FF56086	Cylinder Volume: 31.6 CF
Laboratory: 124 - Plumsteadville - PA	Cylinder Pressure: 2217 PSIG
PGVP Number: A12024	Valve Outlet: 330
Gas Code: H2S,BALN	Certification Date: Sep 04, 2024

Expiration Date: Sep 04, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	41.00 PPM	G1	+/- 1.7% NIST Traceable	08/27/2024, 09/04/2024
NITROGEN	Balance				


CALIBRATION STANDARDS						
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date	
GMIS	122401193440108	CC440120	49.49 PPM HYDROGEN SULFIDE/NITROGEN	+/-1.6%	Sep 28, 2026	
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028	

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Aug 15, 2024

Triad Data Available Upon Request





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33A00Q0	Reference Number:	160-403366847-1A
Cylinder Number:	FF28783	Cylinder Volume:	31.6 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2217 PSIG
PGVP Number:	A12025	Valve Outlet:	330
Gas Code:	H2S,BALN	Certification Date:	Jul 08, 2025

Expiration Date: Jul 08, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	39.98 PPM	G1	+/- 2.0% NIST Traceable	07/01/2025, 07/08/2025
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	122401906919101	CC1077	49.35 PPM HYDROGEN SULFIDE/NITROGEN	1.6%	Dec 21, 2026
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Jun 19, 2025

Triad Data Available Upon Request



Handwritten signature/initials

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - HENDERSON ,	Reference Number: 126-403147050-1
CO	
Part X07NI99C33A0033	Cylinder Volume: 308.0 CF
Number:	
Cylinder FF39589	Cylinder Pressure: 2216 PSIG
Number:	Valve Outlet: 350
Laboratory: 124 - La Porte Mix - TX	
Analysis Oct 09, 2024	
Date:	
Lot Number: 126-403147050-1	
Expiration Date: Oct 09, 2027	

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	20.00 PPM	18.54 PPM	+/-5%
ETHYL BENZENE	20.00 PPM	19.25 PPM	+/-5%
TOLUENE	20.00 PPM	19.40 PPM	+/-5%
M XYLENE	20.00 PPM	19.25 PPM	+/-5%
O XYLENE	20.00 PPM	18.90 PPM	+/-5%
P XYLENE	20.00 PPM	19.17 PPM	+/-5%
NITROGEN	Balance		

Notes: MONTROSE AIR QUALITY SERVICES LLC
PO#: 62293





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E03NI99E33A00K9	Reference Number:	153-403128093-1
Cylinder Number:	EA0037467	Cylinder Volume:	31.6 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	2217 PSIG
PGVP Number:	B72024	Valve Outlet:	660
Gas Code:	NO,NOX,SO2,BALN	Certification Date:	Sep 03, 2024

Expiration Date: Sep 03, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	40.00 PPM	39.48 PPM	G1	+/- 0.6% NIST-Traceable	08/26/2024, 09/03/2024
SULFUR DIOXIDE	40.00 PPM	39.56 PPM	G1	+/- 0.8% NIST Traceable	08/26/2024, 09/03/2024
NITRIC OXIDE	40.00 PPM	39.38 PPM	G1	+/- 0.7% NIST Traceable	08/26/2024, 09/03/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	DCK01201202249	CC750448	49.13 PPM NITRIC OXIDE/NITROGEN	0.5%	May 03, 2026
PRM	12404	APEX1324257	50.04 PPM NITRIC OXIDE/NITROGEN	0.4%	Dec 22, 2023
GMIS	1531022022103	CC517868	4.914 PPM NITROGEN DIOXIDE/NITROGEN	1.6%	Feb 17, 2026
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	1.5%	Feb 17, 2023
GMIS	072120222A114	EB0141223	49.87 PPM SULFUR DIOXIDE/NITROGEN	0.7%	Dec 21, 2026
SRM	12431	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	0.6%	Jun 27, 2023


The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010228 NO LNO	FTIR	Aug 28, 2024
Nicolet iS50 AUP2010228 NO2 impurity	FTIR NO2 impurity	Aug 28, 2024
Nicolet iS50 AUP2010228 SO2 LSO2	FTIR	Aug 22, 2024

Triad Data Available Upon Request

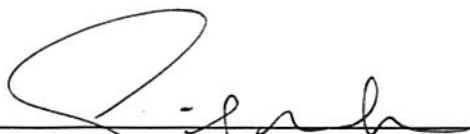


 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E02NI99E33A00Q0	Reference Number: 160-403128091-1
Cylinder Number: FF43945	Cylinder Volume: 31.6 CF
Laboratory: 124 - Plumsteadville - PA	Cylinder Pressure: 2217 PSIG
PGVP Number: A12024	Valve Outlet: 330
Gas Code: H2S,BALN	Certification Date: Sep 04, 2024

Expiration Date: Sep 04, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	40.67 PPM	G1	+/- 2.0% NIST Traceable	08/27/2024, 09/04/2024
NITROGEN	Balance				

CALIBRATION STANDARDS						
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date	
GMIS	122401193440108	CC440120	49.49 PPM HYDROGEN SULFIDE/NITROGEN	+/-1.6%	Sep 28, 2026	
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028	

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Aug 15, 2024

Triad Data Available Upon Request




 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33W0030	Reference Number:	54-403219688-1
Cylinder Number:	D138234	Cylinder Volume:	32.0 CF
Laboratory:	124 - Chicago (SAP) - IL	Cylinder Pressure:	2215 PSIG
PGVP Number:	B12025	Valve Outlet:	660
Gas Code:	NO2,BALN	Certification Date:	Jan 06, 2025

Expiration Date: Jan 06, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NITROGEN DIOXIDE	40.00 PPM	41.69 PPM	G1	+/- 2.1% NIST Traceable	12/27/2024, 01/06/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	1534002024501	CC500127	59.33 PPM NITROGEN DIOXIDE/AIR	+/- 1.8%	Apr 04, 2027
PRM	12438	D153564	59.5 PPM NITROGEN DIOXIDE/AIR	+/- 1.7%	Nov 21, 2024

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR NO2 017707558	FTIR	Jan 03, 2025

Triad Data Available Upon Request

PERMANENT NOTES: OXYGEN ADDED TO MAINTAIN STABILITY.





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33W0030	Reference Number:	153-403375487-1
Cylinder Number:	D285948	Cylinder Volume:	27.4 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	1900 PSIG
PGVP Number:	B72025	Valve Outlet:	660
Gas Code:	NO2,BALN	Certification Date:	Jul 07, 2025

Expiration Date: Jul 07, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NITROGEN DIOXIDE	40.00 PPM	38.47 PPM	G1	+/- 2.0% NIST Traceable	06/30/2025, 07/07/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	1534002024404	CC504401	30.29 PPM NITROGEN DIOXIDE/NITROGEN	1.9%	Apr 04, 2027
PRM	12439	D153559	29.68 PPM NITROGEN DIOXIDE/AIR	1.8%	Nov 22, 2024

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR NO2 018143349	FTIR	Jul 03, 2025

Triad Data Available Upon Request

PERMANENT NOTES: OXYGEN ADDED TO MAINTAIN STABILITY.



[Signature]
Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E03NI99E33A00K9	Reference Number:	153-403128093-1
Cylinder Number:	FF56238	Cylinder Volume:	31.6 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	2217 PSIG
PGVP Number:	B72024	Valve Outlet:	660
Gas Code:	NO,NOX,SO2,BALN	Certification Date:	Sep 03, 2024

Expiration Date: Sep 03, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	40.00 PPM	39.37 PPM	G1	+/- 0.6% NIST Traceable	08/26/2024, 09/03/2024
SULFUR DIOXIDE	40.00 PPM	39.10 PPM	G1	+/- 0.8% NIST Traceable	08/26/2024, 09/03/2024
NITRIC OXIDE	40.00 PPM	39.36 PPM	G1	+/- 0.6% NIST Traceable	08/26/2024, 09/03/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	DCK01201202249	CC750448	49.13 PPM NITRIC OXIDE/NITROGEN	0.5%	May 03, 2026
PRM	12404	APEX1324257	50.04 PPM NITRIC OXIDE/NITROGEN	0.4%	Dec 22, 2023
GMIS	1531022022103	CC517868	4.914 PPM NITROGEN DIOXIDE/NITROGEN	1.6%	Feb 17, 2026
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	1.5%	Feb 17, 2023
GMIS	072120222A114	EB0141223	49.87 PPM SULFUR DIOXIDE/NITROGEN	0.7%	Dec 21, 2026
SRM	12431	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	0.6%	Jun 27, 2023

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010228 NO LNO	FTIR	Aug 28, 2024
Nicolet iS50 AUP2010228 NO2 impurity	FTIR NO2 impurity	Aug 28, 2024
Nicolet iS50 AUP2010228 SO2 LSO2	FTIR	Aug 22, 2024

Triad Data Available Upon Request



Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - HENDERSON ,
CO

Part X07NI99C33A0037

Reference Number: 126-403172475-1

Number:

Cylinder FF17940

Cylinder Volume: 31.6 CF

Number:

Laboratory: 124 - La Porte Mix - TX

Cylinder Pressure: 2217 PSIG

Analysis Nov 18, 2024

Valve Outlet: 350SS

Date:

Lot Number: 126-403172475-1

Expiration Date: Nov 18, 2027

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	2.000 PPM	1.973 PPM	+/- 5%
ETHYL BENZENE	2.000 PPM	1.984 PPM	+/- 5%
M XYLENE	2.000 PPM	1.983 PPM	+/- 5%
O XYLENE	2.000 PPM	1.982 PPM	+/- 5%
P XYLENE	2.000 PPM	1.991 PPM	+/- 5%
TOLUENE	2.000 PPM	1.981 PPM	+/- 5%
NITROGEN	Balance		

Notes: MONTROSE AIR QUALITY SERVICES LLC
PO#: 62293



 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E02NI99E33A00Q0	Reference Number: 160-403366847-1
Cylinder Number: FF42021	Cylinder Volume: 31.6 CF
Laboratory: 124 - Plumsteadville - PA	Cylinder Pressure: 2217 PSIG
PGVP Number: A12025	Valve Outlet: 330
Gas Code: H2S,BALN	Certification Date: Jun 23, 2025

Expiration Date: Jun 23, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	40.39 PPM	G1	+/- 2.0% NIST Traceable	06/17/2025, 06/23/2025
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	122401906919101	CC1077	49.35 PPM HYDROGEN SULFIDE/NITROGEN	1.6%	Dec 21, 2026
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Jun 19, 2025

Triad Data Available Upon Request





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number: E02NI99E33A00Q0	Reference Number: 160-403366847-1
Cylinder Number: FF12847	Cylinder Volume: 31.6 CF
Laboratory: 124 - Plumsteadville - PA	Cylinder Pressure: 2217 PSIG
PGVP Number: A12025	Valve Outlet: 330
Gas Code: H2S,BALN	Certification Date: Jun 23, 2025

Expiration Date: Jun 23, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	40.41 PPM	G1	+/- 2.0% NIST Traceable	06/17/2025, 06/23/2025
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	122401906919101	CC1077	49.35 PPM HYDROGEN SULFIDE/NITROGEN	1.6%	Dec 21, 2026
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Jun 19, 2025

Triad Data Available Upon Request





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E03NI99E33A00K9	Reference Number:	153-403128093-1
Cylinder Number:	EA0037347	Cylinder Volume:	31.6 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	2217 PSIG
PGVP Number:	B72024	Valve Outlet:	660
Gas Code:	NO,NOX,SO2,BALN	Certification Date:	Sep 03, 2024

Expiration Date: Sep 03, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	40.00 PPM	39.50 PPM	G1	+/- 1.3% NIST Traceable	08/26/2024, 09/03/2024
SULFUR DIOXIDE	40.00 PPM	39.51 PPM	G1	+/- 0.8% NIST Traceable	08/26/2024, 09/03/2024
NITRIC OXIDE	40.00 PPM	39.48 PPM	G1	+/- 1.3% NIST Traceable	08/26/2024, 09/03/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	DCK01201202249	CC750448	49.13 PPM NITRIC OXIDE/NITROGEN	0.5%	May 03, 2026
PRM	12404	APEX1324257	50.04 PPM NITRIC OXIDE/NITROGEN	0.4%	Dec 22, 2023
GMIS	1531022022103	CC517868	4.914 PPM NITROGEN DIOXIDE/NITROGEN	1.6%	Feb 17, 2026
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	1.5%	Feb 17, 2023
GMIS	072120222A114	EB0141223	49.87 PPM SULFUR DIOXIDE/NITROGEN	0.7%	Dec 21, 2026
SRM	12431	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	0.6%	Jun 27, 2023

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010228 NO LNO	FTIR	Aug 28, 2024
Nicolet iS50 AUP2010228 NO2 impurity	FTIR NO2 impurity	Aug 28, 2024
Nicolet iS50 AUP2010228 SO2 LSO2	FTIR	Aug 22, 2024

Triad Data Available Upon Request



 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33W0030	Reference Number:	54-403219688-1
Cylinder Number:	D233089	Cylinder Volume:	32.0 CF
Laboratory:	124 - Chicago (SAP) - IL	Cylinder Pressure:	2215 PSIG
PGVP Number:	B12025	Valve Outlet:	660
Gas Code:	NO2,BALN	Certification Date:	Jan 06, 2025

Expiration Date: Jan 06, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NITROGEN DIOXIDE	40.00 PPM	41.78 PPM	G1	+/- 2.1% NIST Traceable	12/27/2024, 01/06/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	1534002024501	CC500127	59.33 PPM NITROGEN DIOXIDE/AIR	+/- 1.8%	Apr 04, 2027
PRM	12438	D153564	59.5 PPM NITROGEN DIOXIDE/AIR	+/- 1.7%	Nov 21, 2024

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR NO2 017707558	FTIR	Jan 03, 2025

Triad Data Available Upon Request

PERMANENT NOTES: OXYGEN ADDED TO MAINTAIN STABILITY.





 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33A00Q0	Reference Number:	160-403128091-1
Cylinder Number:	FF37758	Cylinder Volume:	31.6 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2217 PSIG
PGVP Number:	A12024	Valve Outlet:	330
Gas Code:	H2S,BALN	Certification Date:	Sep 04, 2024

Expiration Date: Sep 04, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	40.52 PPM	G1	+/- 1.6% NIST Traceable	08/27/2024, 09/04/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	122401193440108	CC440120	49.49 PPM HYDROGEN SULFIDE/NITROGEN	+/-1.6%	Sep 28, 2026
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Aug 15, 2024

Triad Data Available Upon Request




 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - HENDERSON , CO	Reference Number: 126-403172475-1
Part X07NI99C33A0037	Cylinder Volume: 31.6 CF
Number: FF660201	Cylinder Pressure: 2217 PSIG
Laboratory: 124 - La Porte Mix - TX	Valve Outlet: 350SS
Analysis Nov 18, 2024	
Date:	
Lot Number: 126-403172475-1	
Expiration Date: Nov 18, 2027	

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	2.000 PPM	1.986 PPM	+/- 5%
ETHYL BENZENE	2.000 PPM	1.997 PPM	+/- 5%
M XYLENE	2.000 PPM	1.996 PPM	+/- 5%
O XYLENE	2.000 PPM	1.995 PPM	+/- 5%
P XYLENE	2.000 PPM	2.004 PPM	+/- 5%
TOLUENE	2.000 PPM	1.998 PPM	+/- 5%
NITROGEN	Balance		

Notes: MONTROSE AIR QUALITY SERVICES LLC
PO#: 62293



W.B.

Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: CERTIFIED STANDARD-SPEC

Customer: MONTROSE AIR QUALITY SERVICES LLC - C264

HENDERSON, CO

Part X07NI99C33A0033

Reference Number: 126-403178702-1

Number:

Cylinder EX0015934

Cylinder Volume: 30.8 CF

Number:

Laboratory: 124 - La Porte Mix - TX

Cylinder Pressure: 2216 PSIG

Analysis Nov 13, 2024

Valve Outlet: 350

Date:

Lot Number: 126-403178702-1

Expiration Date: **Nov 13, 2027**

Product composition verified by direct comparison to calibration standards traceable to N.I.S.T. weights and/or N.I.S.T. Gas Mixture reference materials.

ANALYTICAL RESULTS

Component	Req Conc	Actual Concentration (Mole %)	Analytical Uncertainty
BENZENE	20.00 PPM	20.14 PPM	± 5%
ETHYL BENZENE	20.00 PPM	20.16 PPM	± 5%
TOLUENE	20.00 PPM	20.14 PPM	± 5%
M XYLENE	20.00 PPM	20.13 PPM	± 5%
O XYLENE	20.00 PPM	20.13 PPM	± 5%
P XYLENE	20.00 PPM	20.13 PPM	± 5%
NITROGEN	Balance		

Notes:.

PO NUMBER: 62293



 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33A00Q0	Reference Number:	160-403128091-1
Cylinder Number:	FF56060	Cylinder Volume:	31.6 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2217 PSIG
PGVP Number:	A12024	Valve Outlet:	330
Gas Code:	H2S,BALN	Certification Date:	Sep 04, 2024

Expiration Date: Sep 04, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
HYDROGEN SULFIDE	40.00 PPM	39.75 PPM	G1	+/- 2.0% NIST Traceable	08/27/2024, 09/04/2024
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	122401193440108	CC440120	49.49 PPM HYDROGEN SULFIDE/NITROGEN	+/-1.6%	Sep 28, 2026
PRM	2023050013-1	D133048	50 PPM HYDROGEN SULFIDE/NITROGEN	+/-0.80%	Jul 17, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
AAI-OMA406-AA210275	NDUV	Aug 15, 2024

Triad Data Available Upon Request



Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E03NI99E33A00K9	Reference Number:	153-403128093-1
Cylinder Number:	EA0026117	Cylinder Volume:	31.6 CF
Laboratory:	124 - Tooele (SAP) - UT	Cylinder Pressure:	2217 PSIG
PGVP Number:	B72024	Valve Outlet:	660
Gas Code:	NO,NOX,SO2,BALN	Certification Date:	Sep 03, 2024

Expiration Date: Sep 03, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	40.00 PPM	39.39 PPM	G1	+/- 0.8% NIST Traceable	08/26/2024, 09/03/2024
SULFUR DIOXIDE	40.00 PPM	39.05 PPM	G1	+/- 1.4% NIST Traceable	08/26/2024, 09/03/2024
NITRIC OXIDE	40.00 PPM	39.26 PPM	G1	+/- 0.9% NIST Traceable	08/26/2024, 09/03/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	DCK01201202249	CC750448	49.13 PPM NITRIC OXIDE/NITROGEN	0.5%	May 03, 2026
PRM	12404	APEX1324257	50.04 PPM NITRIC OXIDE/NITROGEN	0.4%	Dec 22, 2023
GMIS	1531022022103	CC517868	4.914 PPM NITROGEN DIOXIDE/NITROGEN	1.6%	Feb 17, 2026
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	1.5%	Feb 17, 2023
GMIS	072120222A114	EB0141223	49.87 PPM SULFUR DIOXIDE/NITROGEN	0.7%	Dec 21, 2026
SRM	12431	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	0.6%	Jun 27, 2023

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010228 NO LNO	FTIR	Aug 28, 2024
Nicolet iS50 AUP2010228 NO2 impurity	FTIR NO2 impurity	Aug 28, 2024
Nicolet iS50 AUP2010228 SO2 LSO2	FTIR	Aug 22, 2024

Triad Data Available Upon Request



 Approved for Release

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Part Number:	E02NI99E33W0030	Reference Number:	54-403219688-1
Cylinder Number:	D202977	Cylinder Volume:	32.0 CF
Laboratory:	124 - Chicago (SAP) - IL	Cylinder Pressure:	2215 PSIG
PGVP Number:	B12025	Valve Outlet:	660
Gas Code:	NO2,BALN	Certification Date:	Jan 06, 2025

Expiration Date: Jan 06, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NITROGEN DIOXIDE	40.00 PPM	41.86 PPM	G1	+/- 2.1% NIST Traceable	12/27/2024, 01/06/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	1534002024501	CC500127	59.33 PPM NITROGEN DIOXIDE/AIR	+/- 1.8%	Apr 04, 2027
PRM	12438	D153564	59.5 PPM NITROGEN DIOXIDE/AIR	+/- 1.7%	Nov 21, 2024

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR NO2 017707558	FTIR	Jan 03, 2025

Triad Data Available Upon Request

PERMANENT NOTES: OXYGEN ADDED TO MAINTAIN STABILITY.




 Approved for Release